

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
 Data File : BM019287.D
 Acq On : 21 Mar 2019 07:40
 Operator : JU/SJ
 Sample : K1943-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 20190124-LOC-1

Quant Time: Mar 21 17:18:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 21 17:06:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	174608	20.00	ng	0.00
21) Naphthalene-d8	10.42	136	725875	20.00	ng	0.00
39) Acenaphthene-d10	14.29	164	465189	20.00	ng	0.00
64) Phenanthrene-d10	17.04	188	1062326	20.00	ng	0.00
76) Chrysene-d12	21.24	240	853952	20.00	ng	0.00
87) Perylene-d12	23.47	264	785949	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	1258015	116.68	ng	0.00
7) Phenol-d6	6.82	99	1642699	104.16	ng	0.00
23) Nitrobenzene-d5	8.80	82	1280778	83.41	ng	0.00
42) 2,4,6-Tribromophenol	15.79	330	888685	129.39	ng	0.00
45) 2-Fluorobiphenyl	12.90	172	2896624	81.00	ng	0.00
79) Terphenyl-d14	19.69	244	4782973	111.19	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019287.D
Acq On : 21 Mar 2019 07:40
Operator : JU/SJ
Sample : K1943-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20190124-LOC-1

Quant Time: Mar 21 17:18:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 21 17:06:23 2019
Response via : Initial Calibration

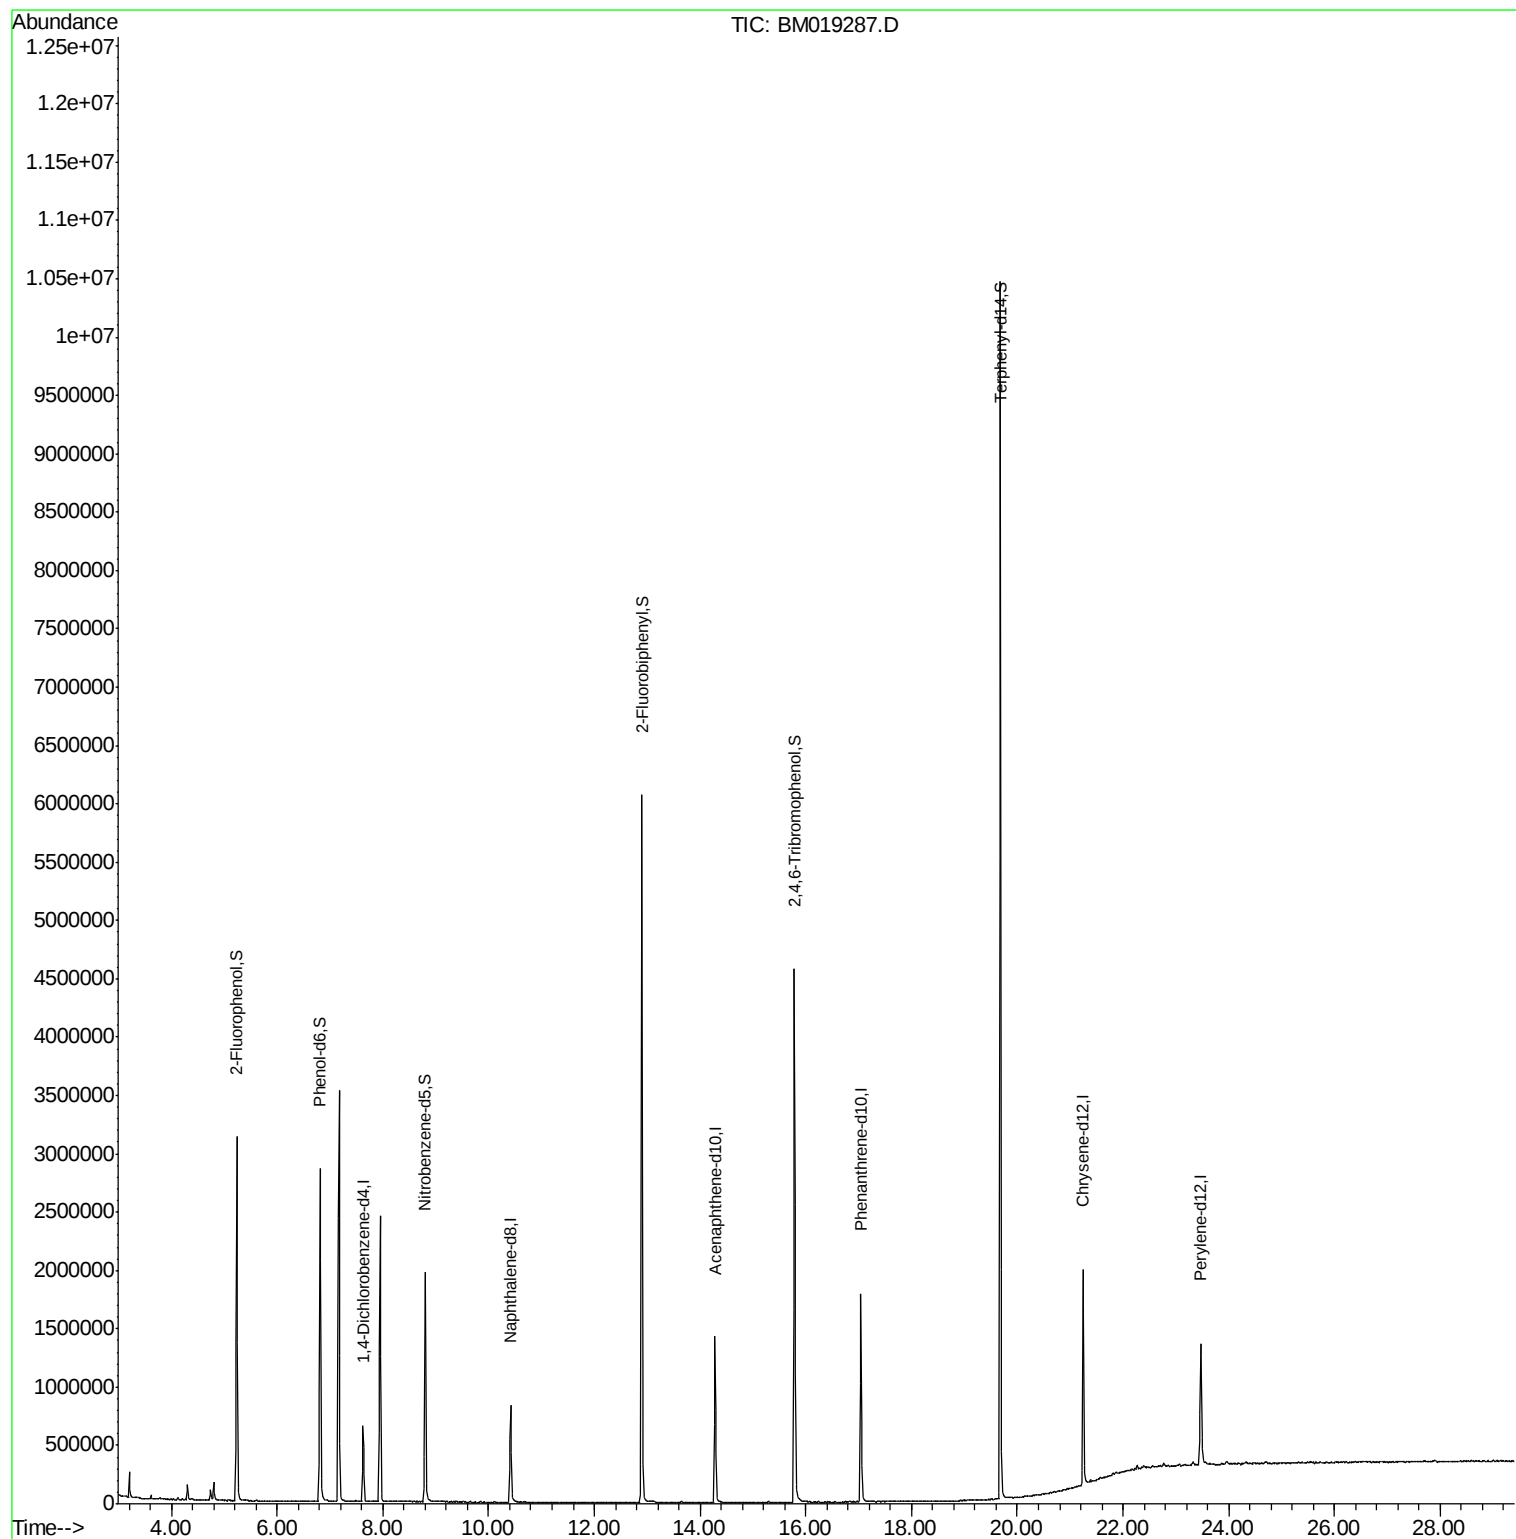




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.63 min Scan# 790
Delta R.T. 0.00 min
Lab File: BM019287.D
Acq: 21 Mar 2019 07:40

Instrument :
BNA_M
ClientSampleId :
20190124-LOC-1

Tot Ion:152 Resp: 174608
Ion Ratio Lower Upper
152 100
150 156.1 123.8 185.6
115 60.7 48.9 73.3




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

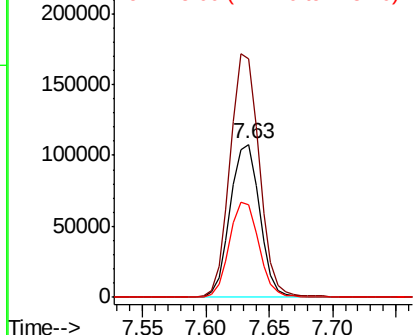



#5


2-Fluorophenol
Concen: 116.680 ng
RT: 5.23 min Scan# 382
Delta R.T. 0.00 min
Lab File: BM019287.D
Acq: 21 Mar 2019 07:40

Tgt Ion:112 Resp: 1258015
Ion Ratio Lower Upper
112 100
64 62.3 50.6 75.8
63 32.0 25.8 38.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

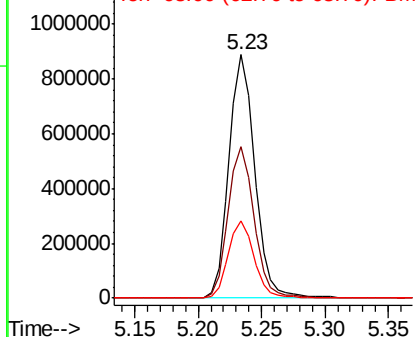



#7

Phenol-d6

Concen: 104.163 ng

RT: 6.82 min Scan# 651

Delta R.T. 0.00 min

Lab File: BM019287.D

Acq: 21 Mar 2019 07:40

Instrument :

BNA_M

ClientSampleId :

20190124-LOC-1


Tot Ion: 99 Resp: 1642699

Ion Ratio Lower Upper

99 100

42 13.9 11.0 16.6




71 37.8 30.1 45.1



Abundance Ion 99.00 (98.70 to 99.70): BM019287.D (-634) (-)

Ion 42.00 (41.70 to 42.70): BM019287.D (-634) (-)

Ion 71.00 (70.70 to 71.70): BM019287.D (-634) (-)

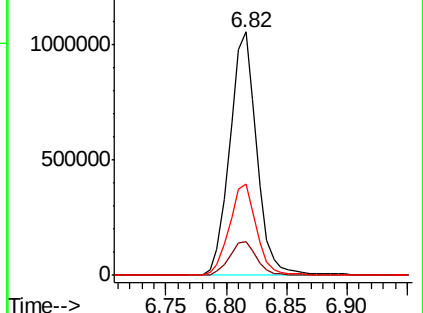

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.42 min Scan# 1263

Delta R.T. 0.00 min

Lab File: BM019287.D

Acq: 21 Mar 2019 07:40

Tgt Ion: 136 Resp: 725875


Ion Ratio Lower Upper

136 100

137 10.6 8.6 12.8

54 6.6 5.5 8.3

68 7.1 6.0 9.0






Abundance Ion 136.00 (135.70 to 136.70): BM019287.D (-1246) (-)

Ion 137.00 (136.70 to 137.70): BM019287.D (-1246) (-)

Ion 54.00 (53.70 to 54.70): BM019287.D (-1246) (-)

Ion 68.00 (67.70 to 68.70): BM019287.D (-1246) (-)



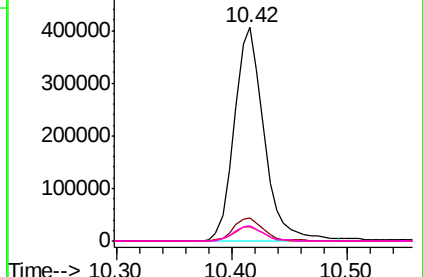



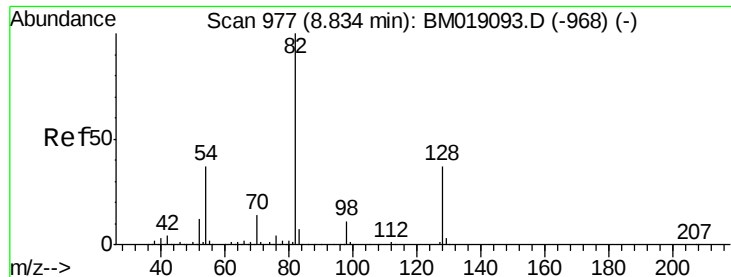

#23
 Nitrobenzene-d5
 Concen: 83.406 ng
 RT: 8.80 min Scan# 988
 Delta R.T. -0.01 min
 Lab File: BM019287.D
 Acq: 21 Mar 2019 07:40




Instrument :
 BNA_M
 ClientSampleId :
 20190124-LOC-1


Tot Ion: 82 Resp: 1280778
 Ion Ratio Lower Upper
 82 100
 128 36.9 30.2 45.4
 54 38.1 30.2 45.2

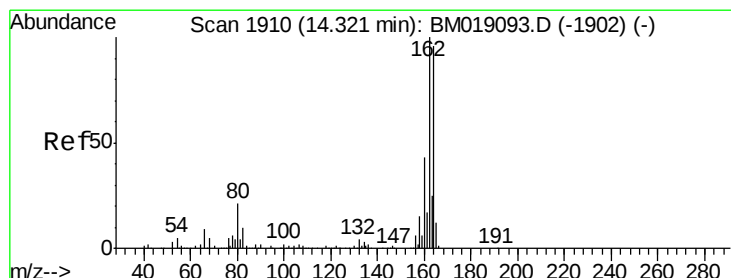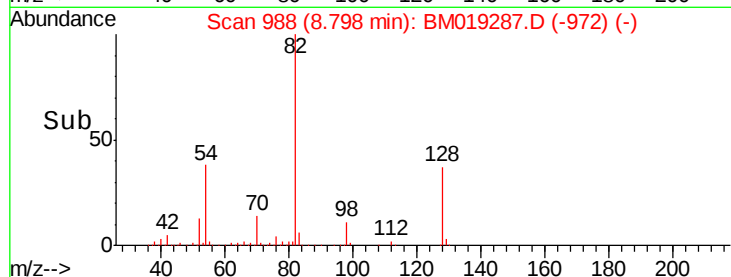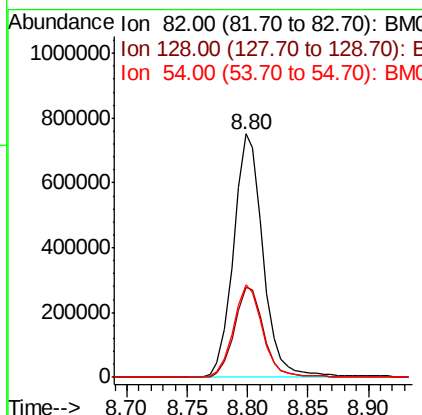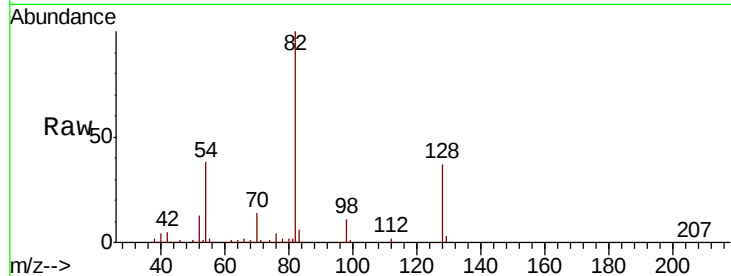

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.29 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BM019287.D
 Acq: 21 Mar 2019 07:40

Tgt Ion:164 Resp: 465189
 Ion Ratio Lower Upper
 164 100
 162 104.2 84.1 126.1
 160 46.1 36.5 54.7

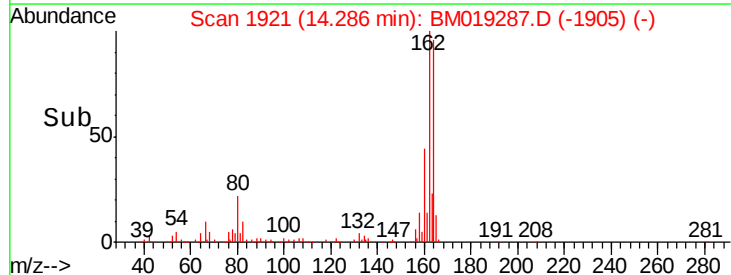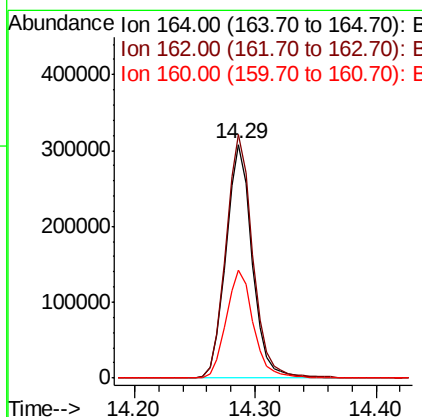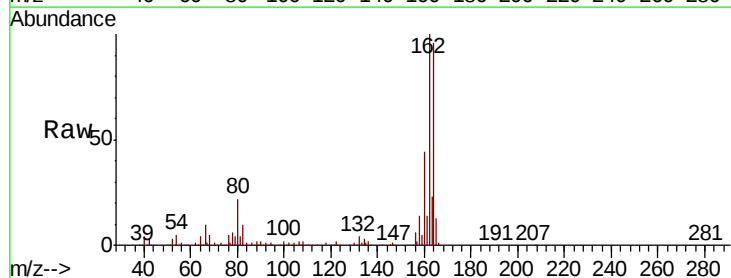




#42
 2,4,6-Tribromophenol
 Concen: 129.388 ng
 RT: 15.79 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: BM019287.D
 Acq: 21 Mar 2019 07:40

Instrument :
 BNA_M
 ClientSampleId :
 20190124-LOC-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.6	116.4
141	32.7	25.7	38.5



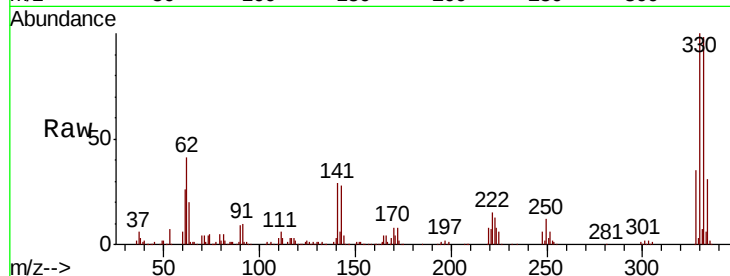


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

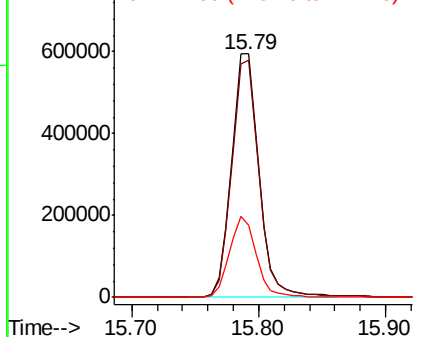

#45
 2-Fluorobiphenyl
 Concen: 80.995 ng
 RT: 12.90 min Scan# 1685
 Delta R.T. -0.01 min
 Lab File: BM019287.D
 Acq: 21 Mar 2019 07:40

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.0	43.4
170	23.2	18.9	28.3






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E




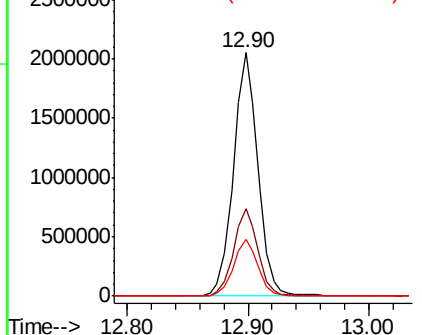




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.04 min Scan# 2390
Delta R.T. 0.00 min
Lab File: BM019287.D
Acq: 21 Mar 2019 07:40




Instrument :
BNA_M
ClientSampleId :
20190124-LOC-1


Tot Ion:188 Resp: 1062326
Ion Ratio Lower Upper
188 100
94 9.8 8.7 13.1
80 11.7 9.8 14.8

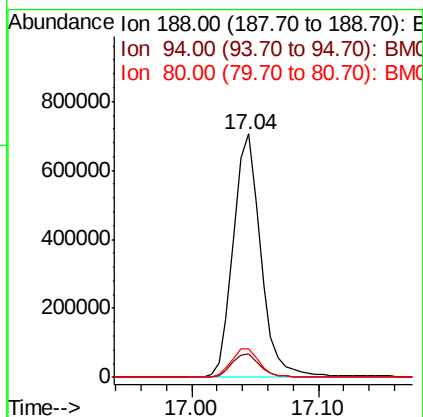

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.24 min Scan# 3104
Delta R.T. -0.01 min
Lab File: BM019287.D
Acq: 21 Mar 2019 07:40

Tgt Ion:240 Resp: 853952
Ion Ratio Lower Upper
240 100
120 12.0 9.2 13.8
236 25.4 20.3 30.5

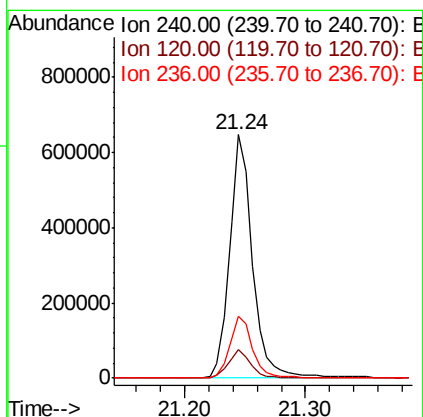

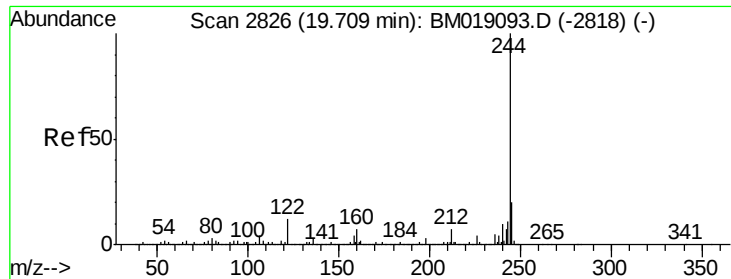

#79

Terphenyl-d14

Concen: 111.192 ng

RT: 19.69 min Scan# 2839

Delta R.T. 0.00 min

Lab File: BM019287.D

Acq: 21 Mar 2019 07:40

Instrument :

BNA_M

ClientSampleId :

20190124-LOC-1


Tot Ion:244 Resp: 4782973

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.2




122 10.9 9.6 14.4

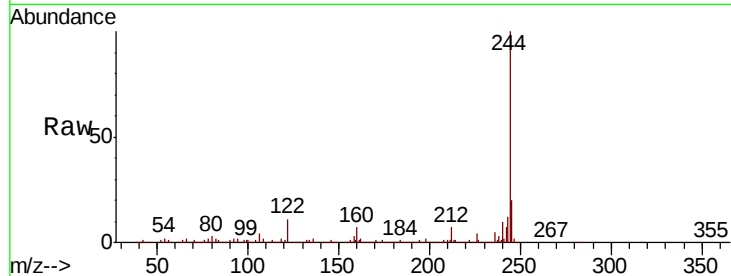

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

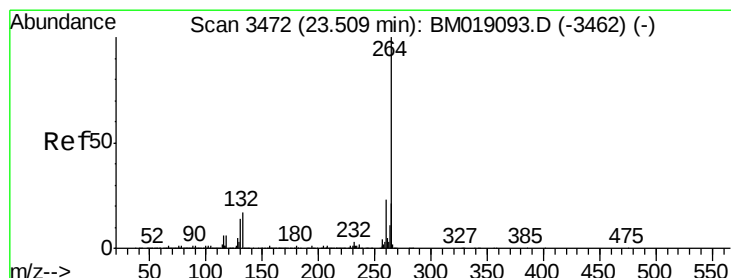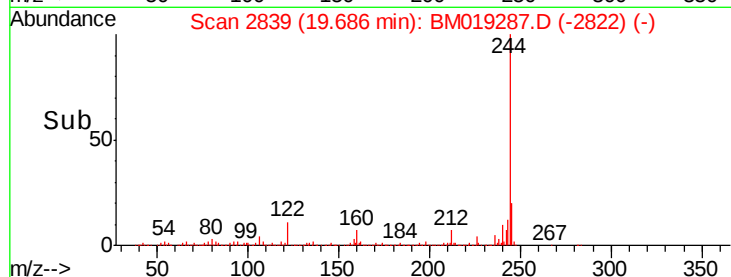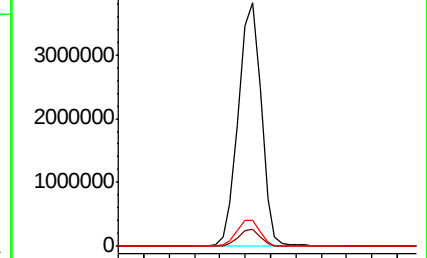

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.47 min Scan# 3483

Delta R.T. 0.00 min

Lab File: BM019287.D

Acq: 21 Mar 2019 07:40


Tgt Ion:264 Resp: 785949

Ion Ratio Lower Upper

264 100

260 23.0 19.0 28.4

265 21.2 17.6 26.4

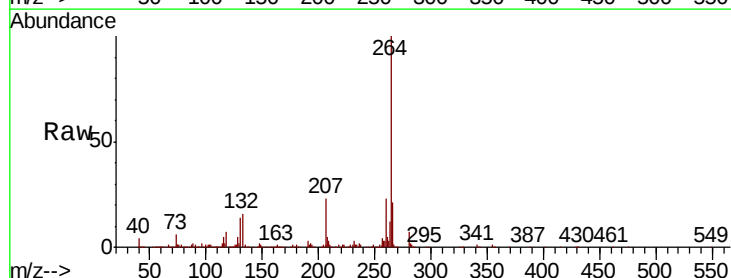

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

