

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
 Data File : BM019264.D
 Acq On : 20 Mar 2019 16:31
 Operator : JU/SJ
 Sample : PB118000BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB118000BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	376	382	398	rBV	3368761	4902498	41.33%	8.081%
2	6.816	644	651	672	rBV	3458383	5482791	46.22%	9.038%
3	7.169	704	711	728	rBV	3612930	5574359	46.99%	9.189%
4	7.634	784	790	800	rBV	645577	1015006	8.56%	1.673%
5	7.951	836	844	855	rBV	2372365	3873721	32.66%	6.385%
6	8.804	981	989	1008	rBV	1769206	3119157	26.30%	5.142%
7	10.416	1257	1263	1288	rVB	725053	1397851	11.78%	2.304%
8	12.904	1679	1686	1708	rBV	5587020	8210389	69.22%	13.534%
9	14.292	1915	1922	1934	rBV2	1310022	2087584	17.60%	3.441%
10	15.792	2170	2177	2198	rBV	4400460	6371398	53.71%	10.503%
11	17.045	2384	2390	2406	rBV2	1591030	2464722	20.78%	4.063%
12	19.686	2833	2839	2856	rBV	9875814	11861637	100.00%	19.553%
13	21.250	3100	3105	3118	rBV	1669700	2331255	19.65%	3.843%
14	23.474	3477	3483	3495	rBV	976023	1972869	16.63%	3.252%


Sum of corrected areas: 60665237

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019264.D
Acq On : 20 Mar 2019 16:31
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118000BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

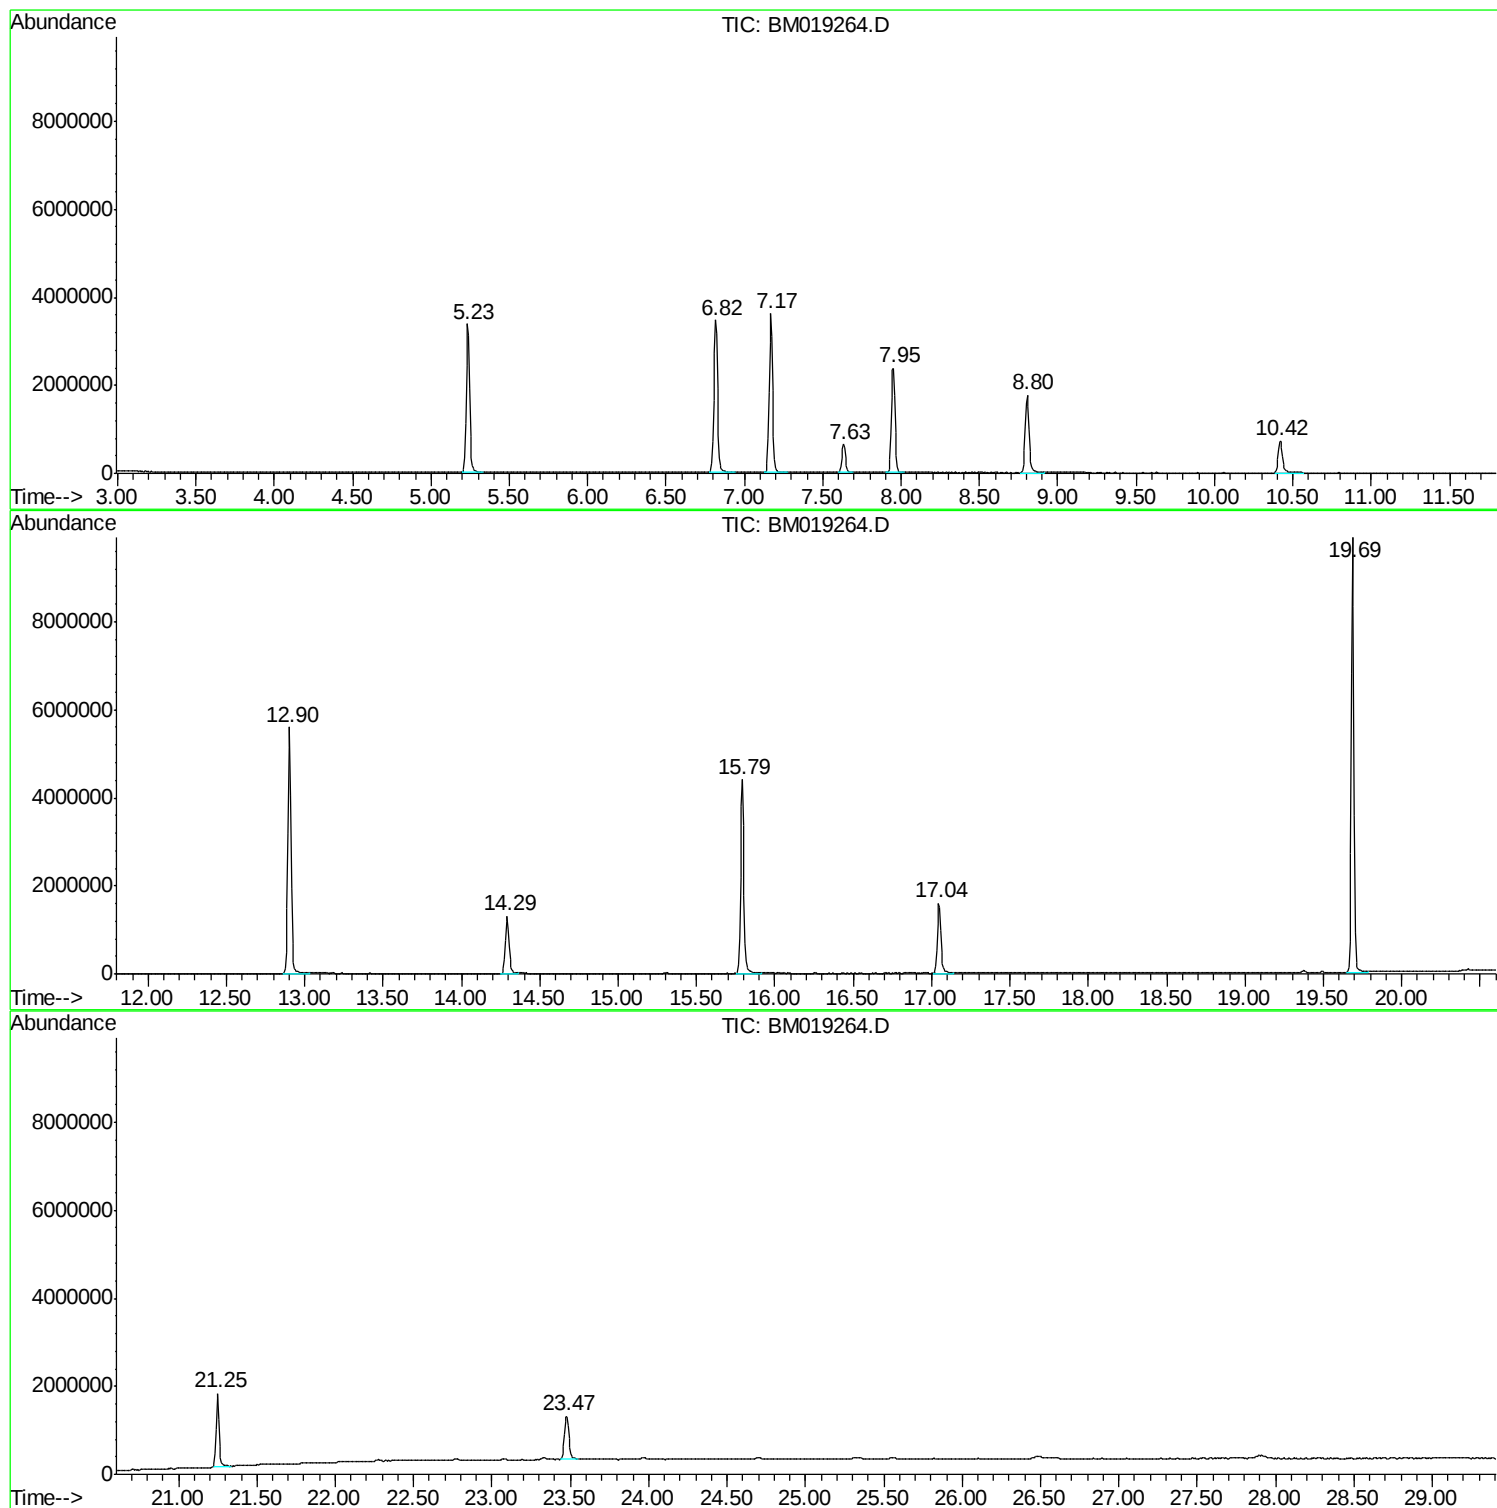

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019264.D
Acq On : 20 Mar 2019 16:31
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118000BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.17 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.17	109.84 ng	5574360	1,4-Dichlorobenzene-d4	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		Xenon	132	Xe	007440-63-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

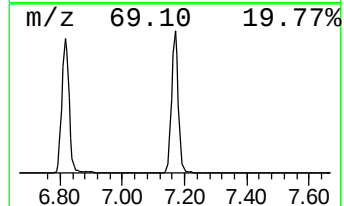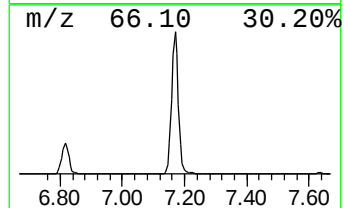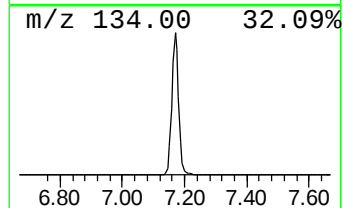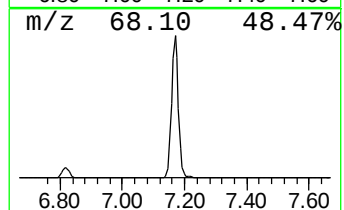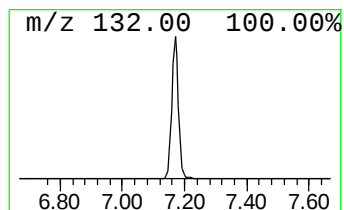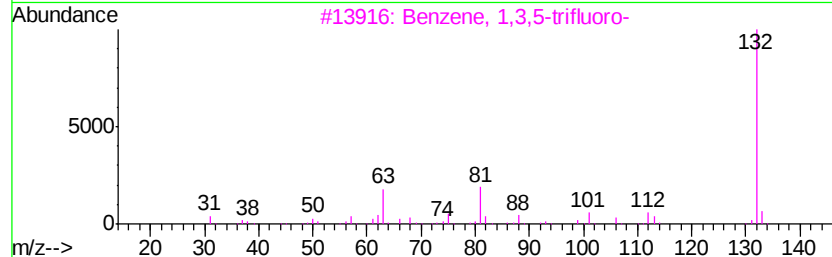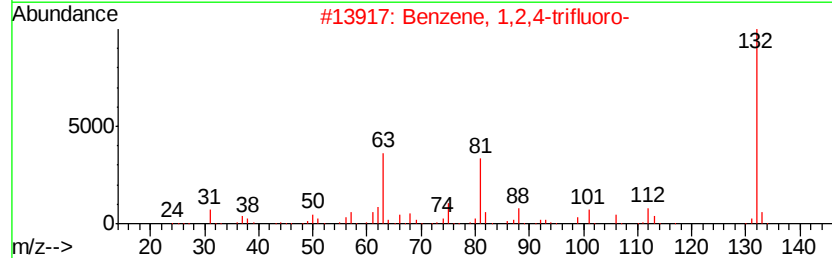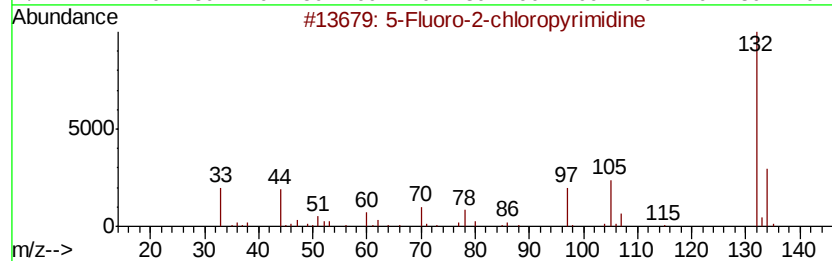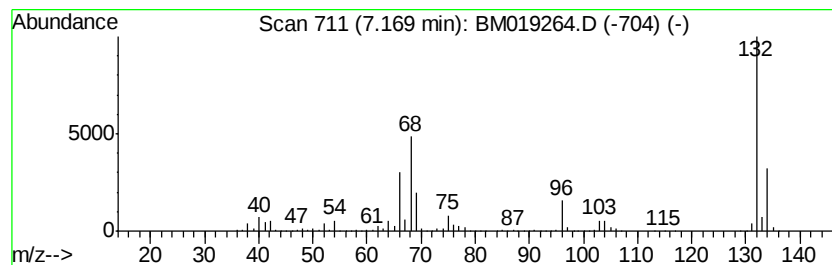

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032019\
Data File : BM019264.D
Acq On : 20 Mar 2019 16:31
Operator : JU/SJ
Sample : PB118000BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118000BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.17	7.17	109.8	ng	5574360	1	7.63	1015010	20.0