

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
 Data File : BM019274.D
 Acq On : 20 Mar 2019 22:35
 Operator : JU/SJ
 Sample : K1964-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TW-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	376	382	393	rBV	1798689	2591846	18.49%	3.833%
2	6.816	644	651	667	rBV	1095500	1859384	13.27%	2.750%
3	7.169	704	711	728	rBV	3739444	5796647	41.36%	8.573%
4	7.634	784	790	799	rBV	789270	1234979	8.81%	1.826%
5	7.951	835	844	854	rBV	2957238	4859562	34.68%	7.187%
6	8.804	981	989	1007	rBV	2636032	4360520	31.12%	6.449%
7	10.416	1255	1263	1283	rBV	1068973	1924028	13.73%	2.845%
8	12.904	1678	1686	1701	rBV	7603175	11043089	78.80%	16.331%
9	14.292	1915	1922	1930	rBV2	1796551	2779559	19.83%	4.111%
10	15.792	2171	2177	2192	rBV	6220447	8712624	62.17%	12.885%
11	17.045	2384	2390	2401	rBV2	2140391	3151900	22.49%	4.661%
12	17.933	2537	2541	2546	rBV	117372	179935	1.28%	0.266%
13	19.686	2833	2839	2859	rBV	11627058	14013966	100.00%	20.725%
14	20.951	3051	3054	3060	rVB2	108446	142983	1.02%	0.211%
15	21.245	3100	3104	3116	rBV	1906715	2594331	18.51%	3.837%
16	23.474	3477	3483	3495	rVB	1228917	2373670	16.94%	3.510%


Sum of corrected areas: 67619023

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019274.D
Acq On : 20 Mar 2019 22:35
Operator : JU/SJ
Sample : K1964-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

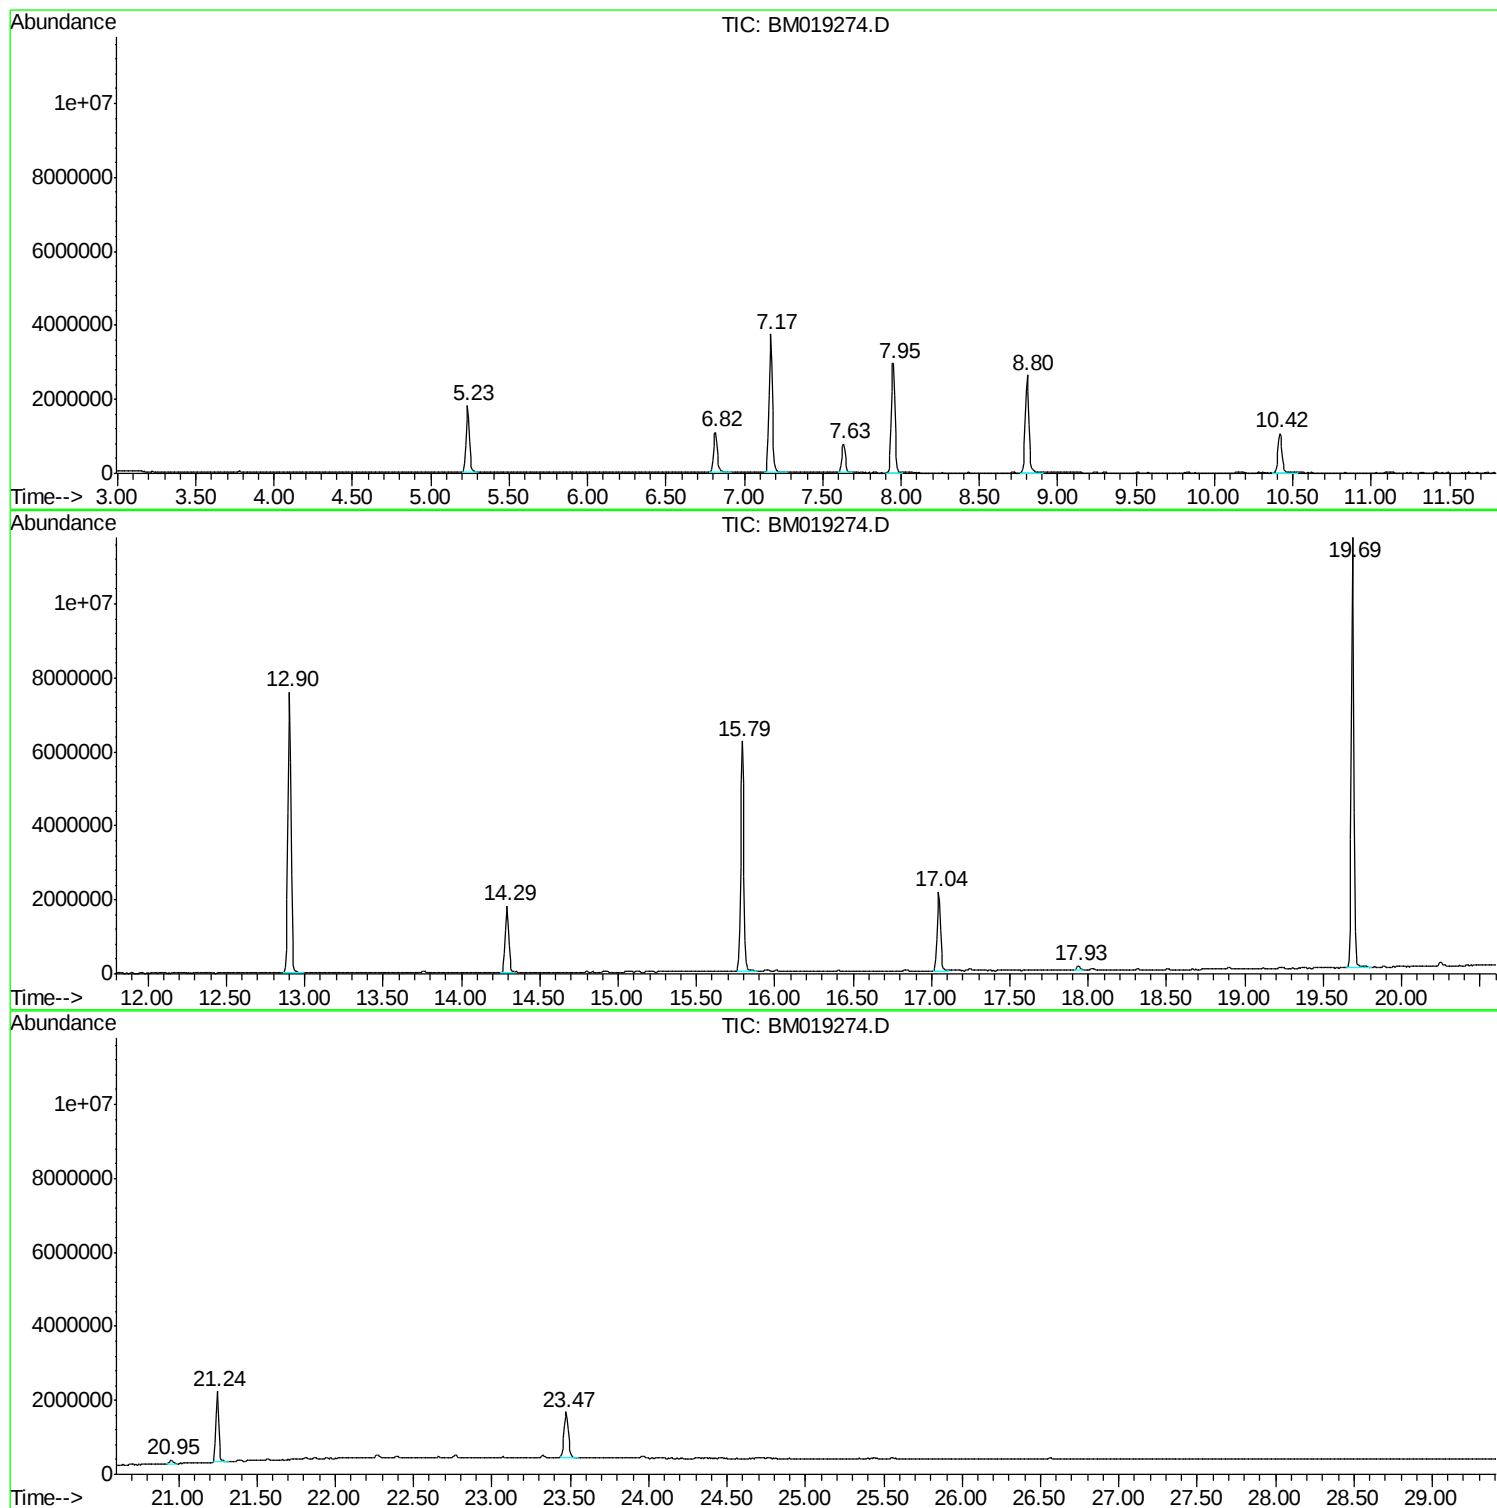

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019274.D
Acq On : 20 Mar 2019 22:35
Operator : JU/SJ
Sample : K1964-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.17 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.17	93.87 ng	5796650	1,4-Dichlorobenzene-d4	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9
5		Xenon	132	Xe	007440-63-3	9

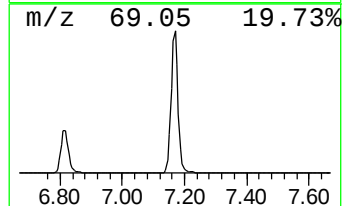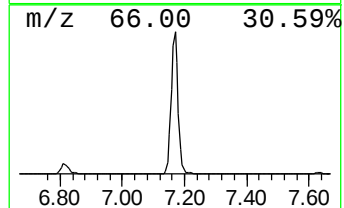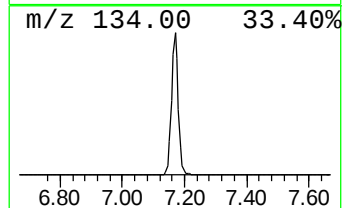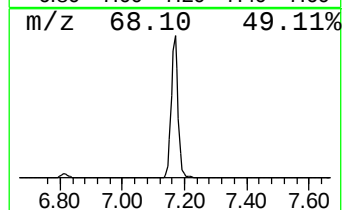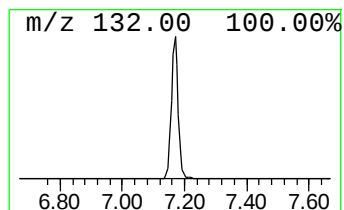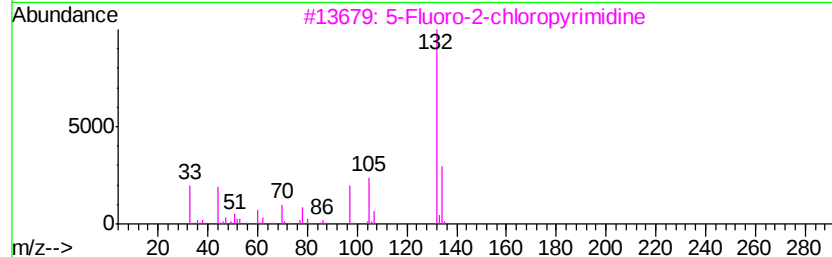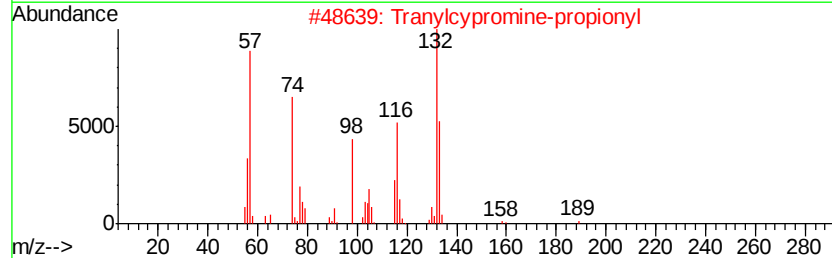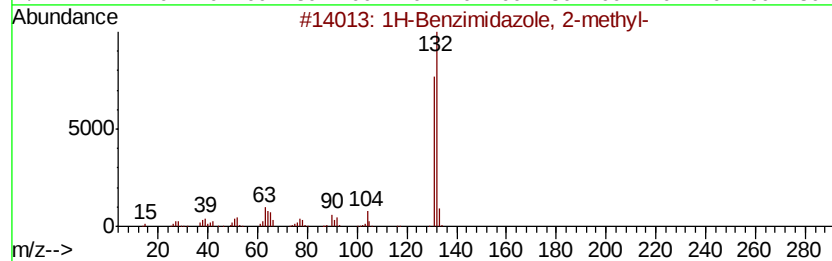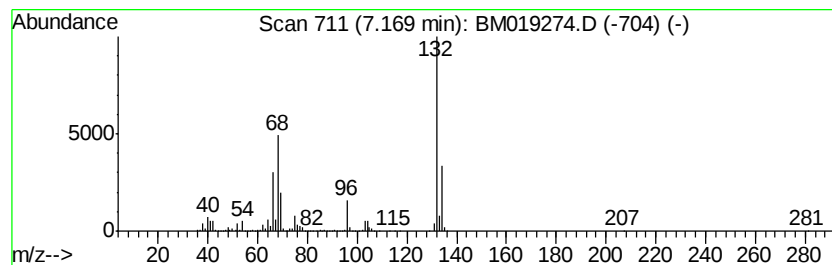

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032019\
Data File : BM019274.D
Acq On : 20 Mar 2019 22:35
Operator : JU/SJ
Sample : K1964-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TW-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.17	7.17	93.9	ng	5796650	1	7.63	1234980	20.0