

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
 Data File : BM019287.D
 Acq On : 21 Mar 2019 07:40
 Operator : JU/SJ
 Sample : K1943-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 20190124-LOC-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	33	37	47	rBV	218956	258007	1.95%	0.408%
2	4.304	221	224	233	rBV	123543	159916	1.21%	0.253%
3	4.798	304	308	319	rVB	149646	222447	1.68%	0.352%
4	5.234	376	382	399	rBV	3121492	4461681	33.69%	7.054%
5	6.816	644	651	670	rBV	2852499	4533875	34.24%	7.168%
6	7.169	703	711	726	rBV	3519625	5575389	42.10%	8.815%
7	7.628	783	789	799	rBV	653766	1060617	8.01%	1.677%
8	7.945	835	843	854	rBV	2448130	3845049	29.04%	6.079%
9	8.798	981	988	1004	rBV	1968062	3386454	25.57%	5.354%
10	10.416	1256	1263	1275	rBV	832385	1491040	11.26%	2.357%
11	12.898	1678	1685	1700	rBV	6064913	8593495	64.89%	13.586%
12	14.286	1914	1921	1933	rBV2	1423137	2270705	17.15%	3.590%
13	15.786	2170	2176	2195	rBV	4569335	6836815	51.63%	10.809%
14	17.045	2383	2390	2406	rBV	1787521	2731991	20.63%	4.319%
15	19.686	2833	2839	2856	rBV	10431676	13242348	100.00%	20.936%
16	21.244	3099	3104	3118	rBV	1853602	2530429	19.11%	4.001%
17	23.474	3477	3483	3495	rVB	1023660	2051067	15.49%	3.243%


Sum of corrected areas: 63251325

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019287.D
Acq On : 21 Mar 2019 07:40
Operator : JU/SJ
Sample : K1943-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
20190124-LOC-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

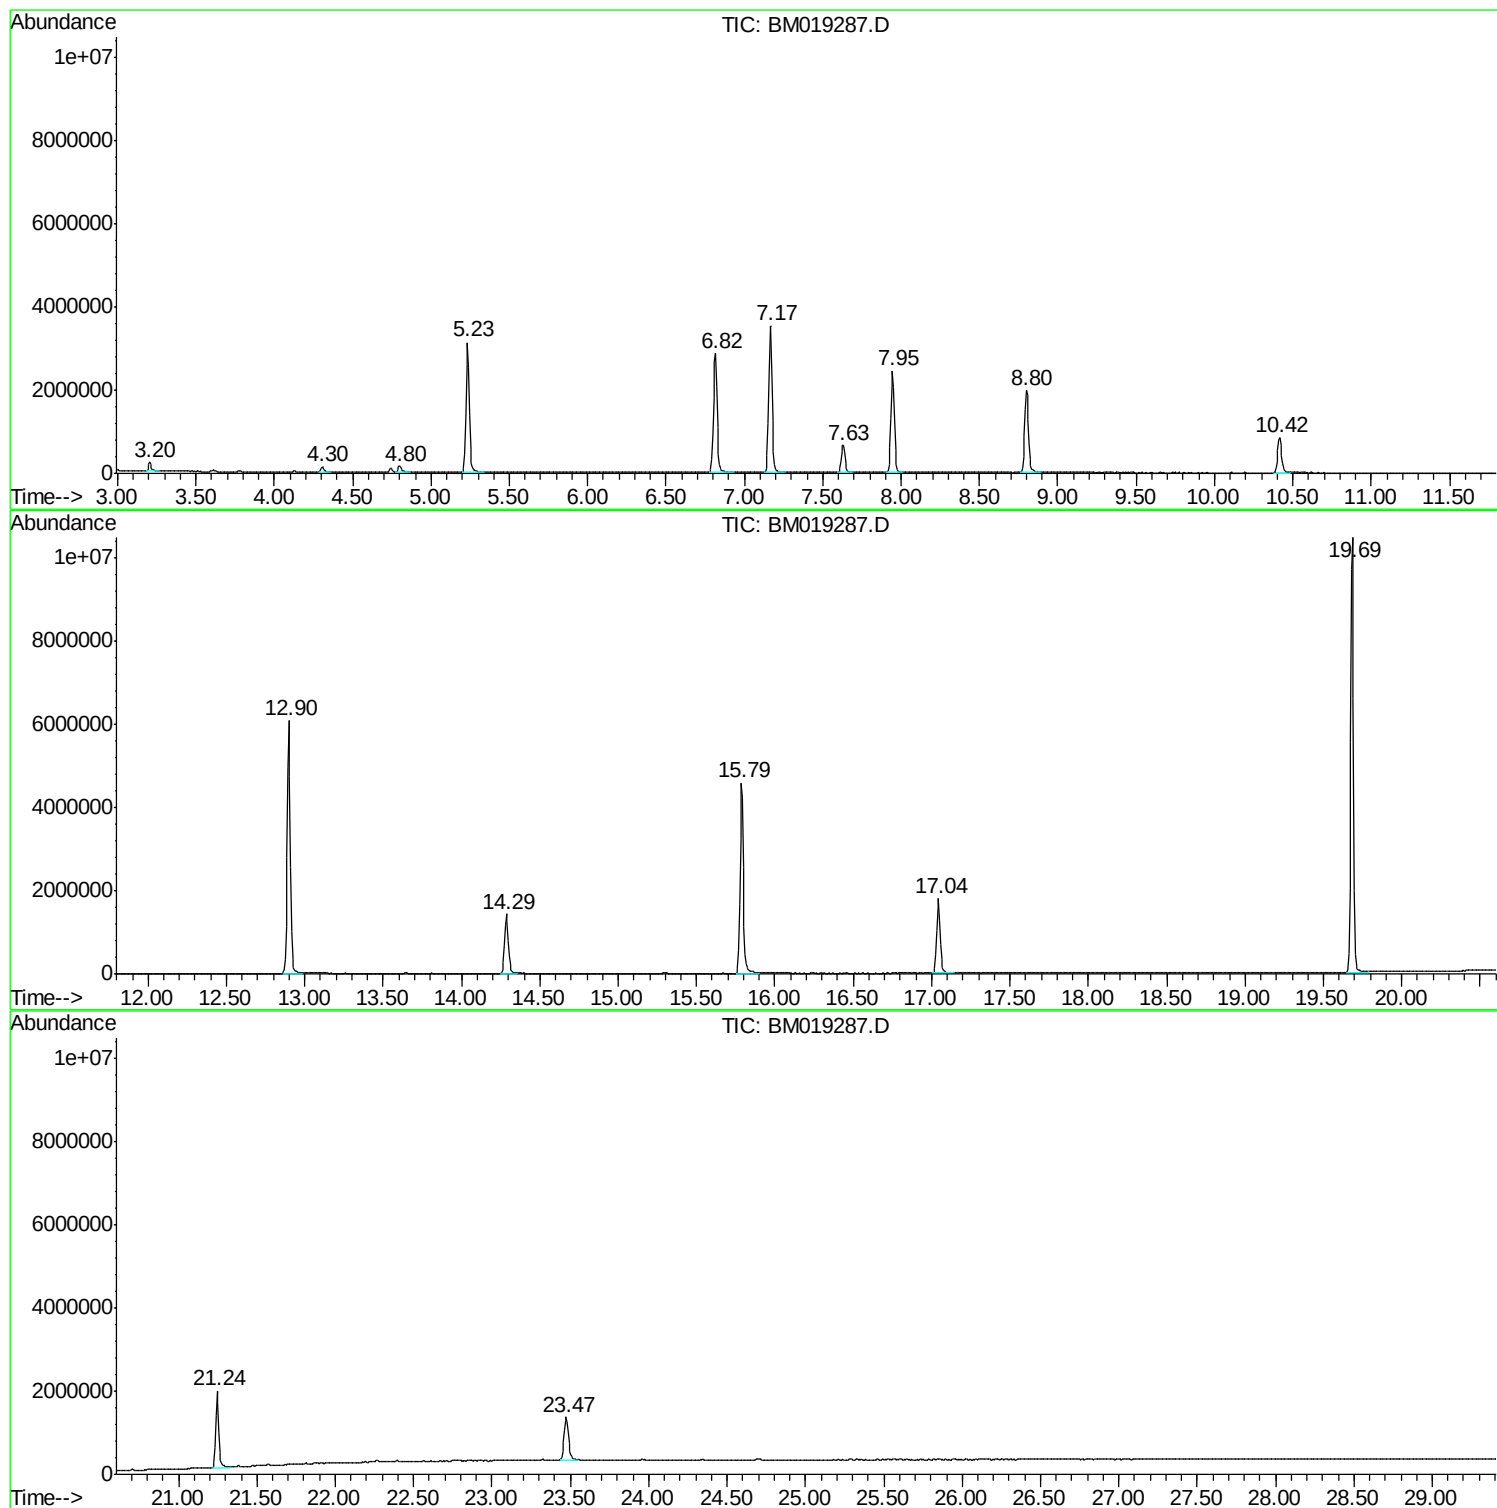

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032019\
Data_File : BM019287.D
Acq_On : 21-Mar-2019 07:400
Operator : JU/SJJ
Sample : K1943-111
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
20190124-LOC-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
