


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
Data File : BM019261.D
Acq On : 20 Mar 2019 14:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 11 17:30:46 2019

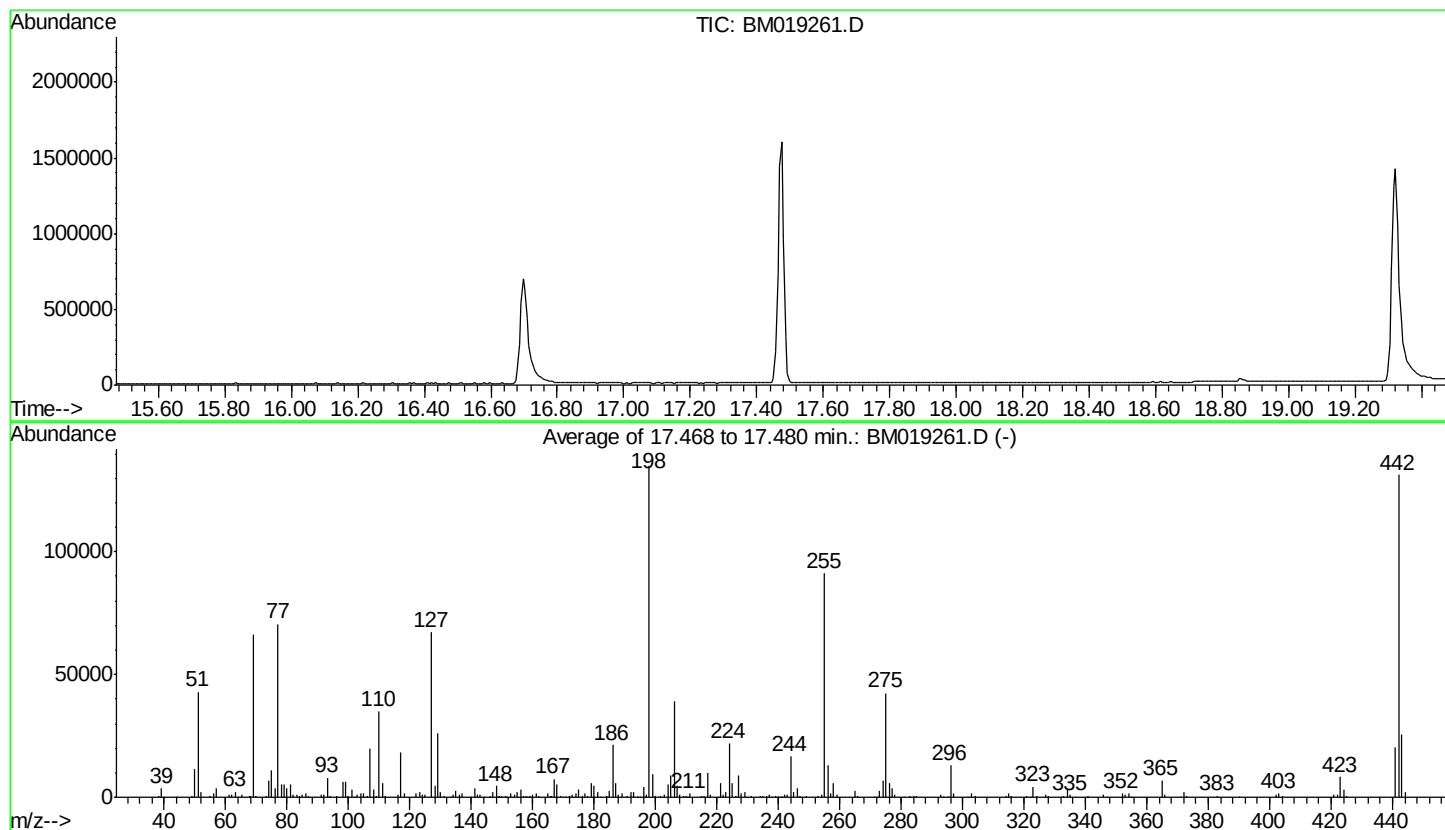

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	42909	PASS
68	69	0.00	2	1.1	741	PASS
69	198	0.00	100	48.9	66114	PASS
70	69	0.00	2	0.5	308	PASS
127	198	10	80	49.7	67138	PASS
197	198	0.00	2	0.7	973	PASS
198	198	100	100	100.0	135130	PASS
199	198	5	9	7.0	9479	PASS
275	198	10	60	31.4	42405	PASS
365	198	1	100	4.8	6551	PASS
441	198	0.01	100	15.2	20581	PASS
442	198	50	100	97.2	131394	PASS
443	442	15	24	19.3	25349	PASS