


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032019\
 Data File : BM019280.D
 Acq On : 21 Mar 2019 03:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

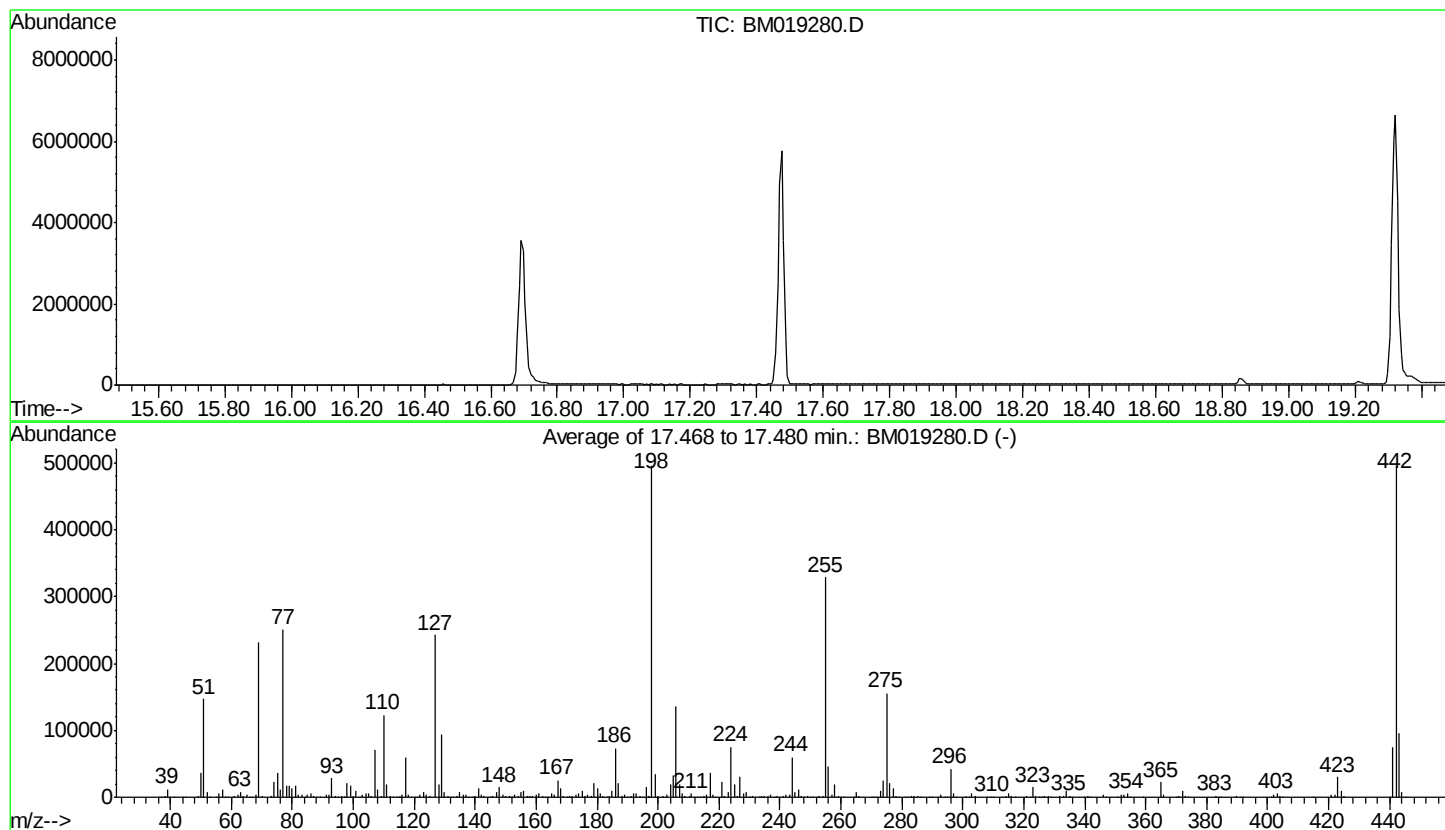

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	147208	PASS
68	69	0.00	2	1.8	4073	PASS
69	198	0.00	100	46.8	231893	PASS
70	69	0.00	2	0.5	1174	PASS
127	198	10	80	48.9	242752	PASS
197	198	0.00	2	0.4	2055	PASS
198	198	100	100	100.0	495957	PASS
199	198	5	9	6.8	33658	PASS
275	198	10	60	31.3	155109	PASS
365	198	1	100	4.5	22133	PASS
441	198	0.01	100	15.0	74344	PASS
442	198	50	100	99.8	495210	PASS
443	442	15	24	19.4	96010	PASS