

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025669.D
 Acq On : 20 Mar 2020 20:05
 Operator : CG/JU
 Sample : L1835-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D81

Quant Time: Mar 20 23:26:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 23:10:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	148542	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	608020	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	367678	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	772982	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	801753	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	879963	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.14	96	18013	5.09	ng/uL	0.00
5) Phenol-d5	6.76	99	87088	7.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	186622	27.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	231111	24.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	153963	15.98	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	137045	30.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	141036	29.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	255185	25.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	22469	1.97	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	831206	29.75	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1019642	30.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	33940	6.38	ng/ul	0.00
58) Fluorene-d10	15.22	176	772351	31.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	119311	25.30	ng/ul	0.00
71) Anthracene-d10	17.06	188	1390346	38.51	ng/ul	0.00
79) Pyrene-d10	19.36	212	1468646	38.14	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1797448	39.90	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	65978	2.268	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025669.D
Acq On : 20 Mar 2020 20:05
Operator : CG/JU
Sample : L1835-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D81

Quant Time: Mar 20 23:26:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 23:10:07 2020
Response via : Initial Calibration

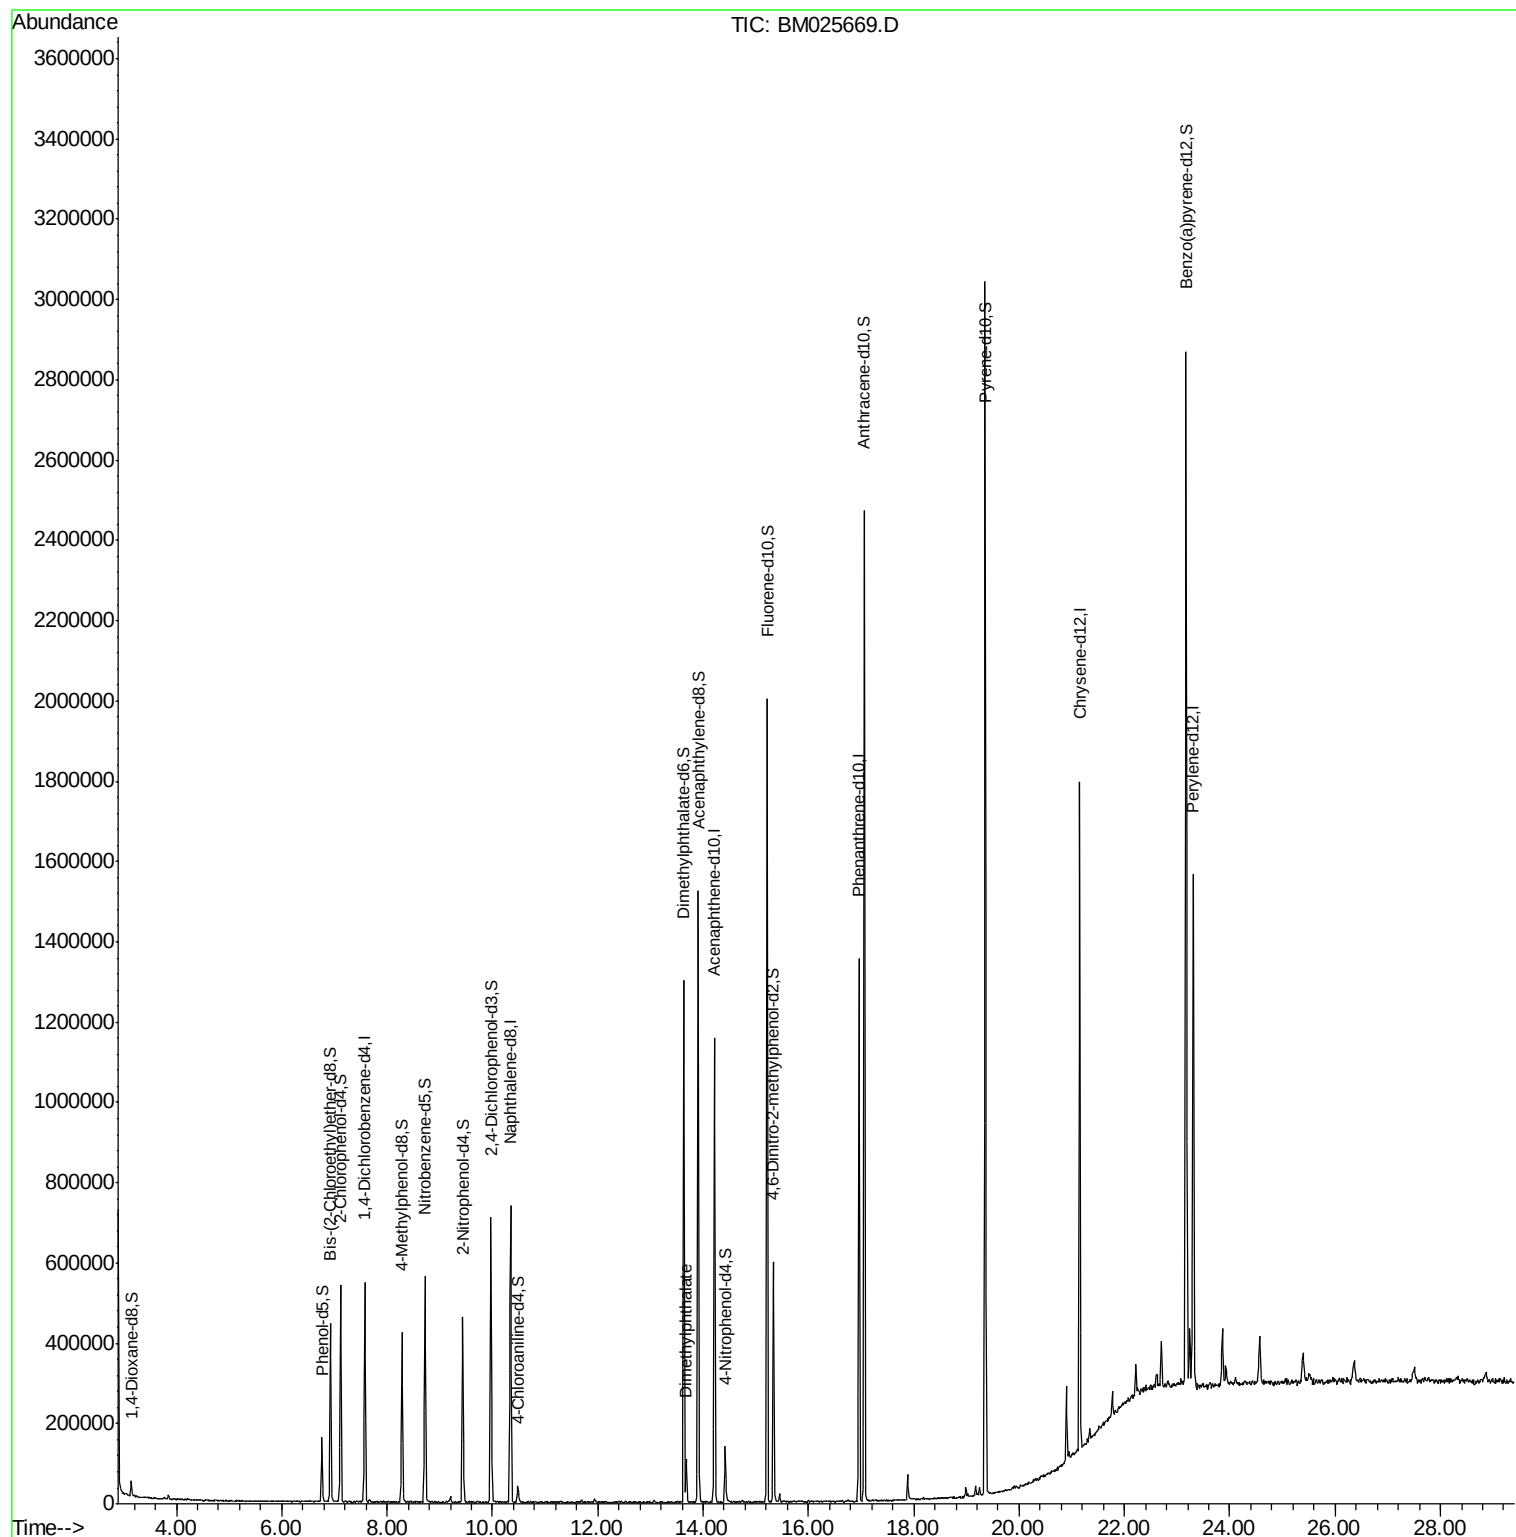

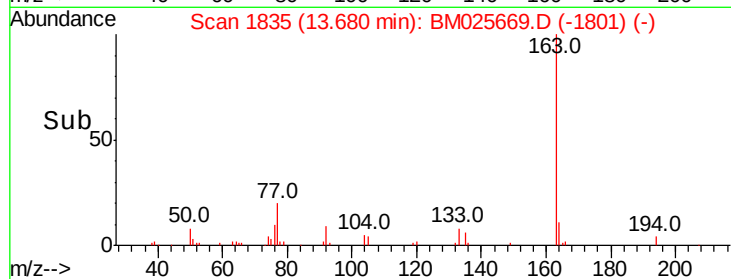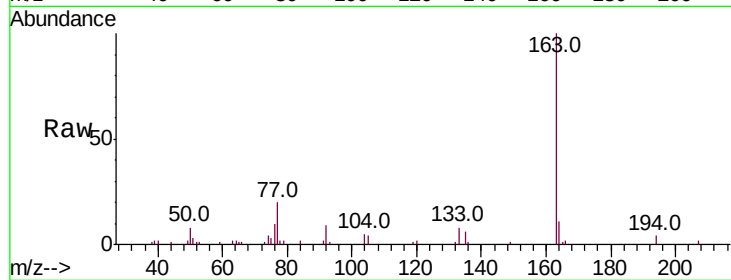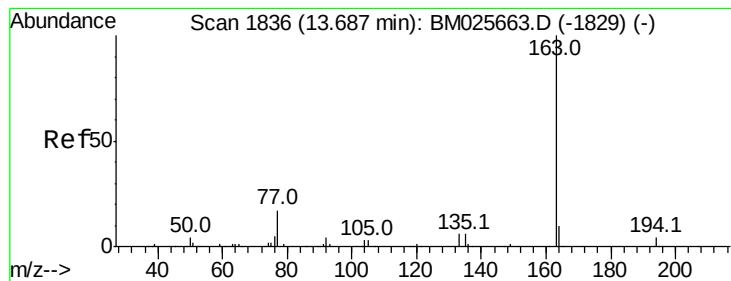

#45

Dimethylphthalate

Concen: 2.268 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BM025669.D

Acq: 20 Mar 2020 20:05

Instrument :

BNA_M

ClientSampleId :

C0D81

Tot Ion:163 Resp: 65978

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 10.9 8.2 12.4

