

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025673.D
 Acq On : 20 Mar 2020 22:31
 Operator : CG/JU
 Sample : L1835-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DJ1

Quant Time: Mar 20 23:53:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 23:10:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	184231	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	774185	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	468530	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	976831	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1020374	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1143999	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.14	96	19844	4.52	ng/uL	0.00
5) Phenol-d5	6.76	99	83088	5.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	224261	27.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	267784	22.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	165562	13.86	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	169565	29.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	182146	29.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	320520	25.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	28287	1.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1139626	32.00	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1342721	31.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	33371	4.92	ng/ul	0.00
58) Fluorene-d10	15.22	176	973187	31.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	139857	23.47	ng/ul	0.00
71) Anthracene-d10	17.06	188	1563173	34.26	ng/ul	0.00
79) Pyrene-d10	19.36	212	1677236	34.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2048740	34.98	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	153715	4.147	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025673.D
Acq On : 20 Mar 2020 22:31
Operator : CG/JU
Sample : L1835-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DJ1

Quant Time: Mar 20 23:53:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 23:10:07 2020
Response via : Initial Calibration

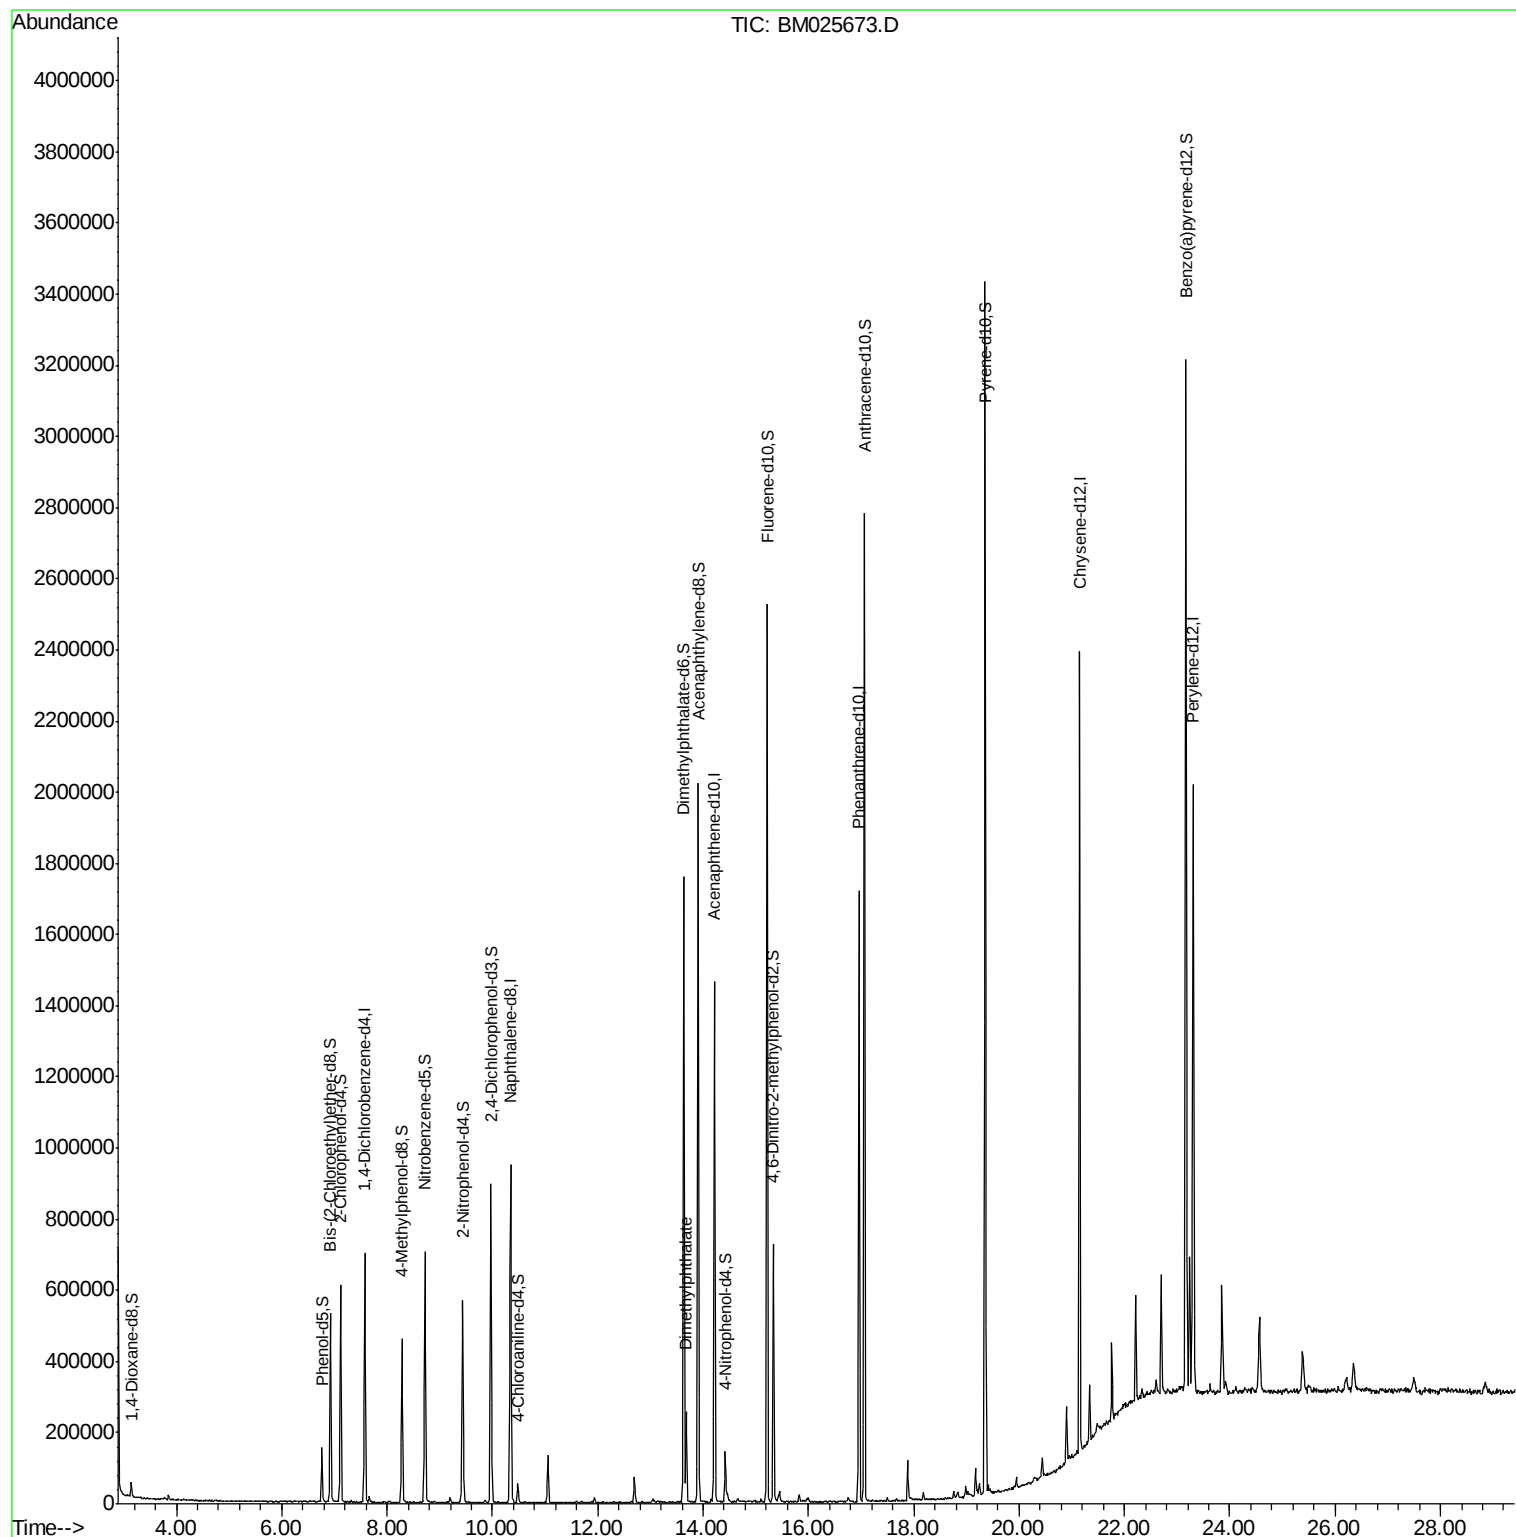

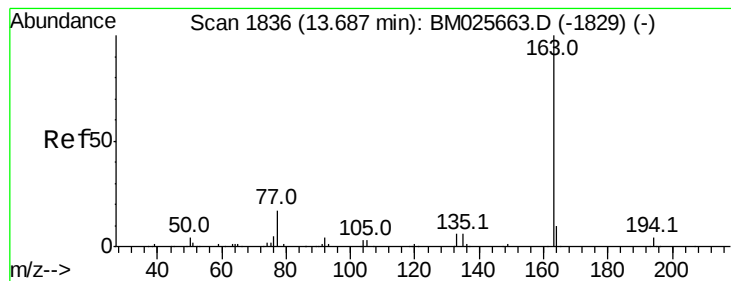

#45

Dimethylphthalate

Concen: 4.147 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BM025673.D

Acq: 20 Mar 2020 22:31

Instrument :

BNA_M

ClientSampleId :

C0DJ1


Tot Ion:163 Resp: 153715

Ion Ratio Lower Upper

163 100

194 5.0 3.5 5.3

164 10.0 8.2 12.4

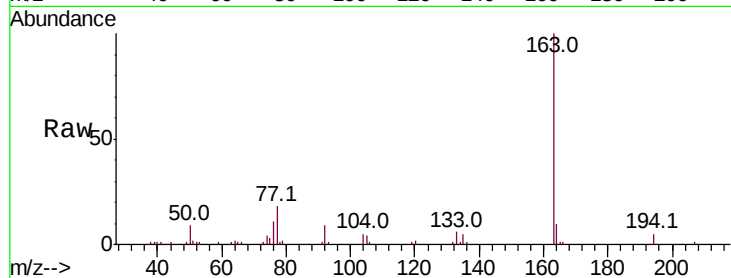

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

