

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025678.D
 Acq On : 21 Mar 2020 01:33
 Operator : CG/JU
 Sample : L1835-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DJ6

Quant Time: Mar 21 02:28:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 23:10:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	240858	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1005041	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	620430	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1305986	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1344978	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1479371	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	16295	2.84	ng/uL	0.00
5) Phenol-d5	6.76	99	107255	5.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	271837	25.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	331130	21.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	203782	13.05	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	204705	27.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	221553	27.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	387329	23.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	34549	1.83	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1295343	27.47	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1547936	27.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	47825	5.33	ng/ul	0.00
58) Fluorene-d10	15.21	176	1169575	28.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	188109	23.61	ng/ul	0.00
71) Anthracene-d10	17.06	188	1996240	32.73	ng/ul	0.00
79) Pyrene-d10	19.36	212	2129611	32.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2515779	33.22	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	117099	2.386	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025678.D
Acq On : 21 Mar 2020 01:33
Operator : CG/JU
Sample : L1835-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DJ6

Quant Time: Mar 21 02:28:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 23:10:07 2020
Response via : Initial Calibration

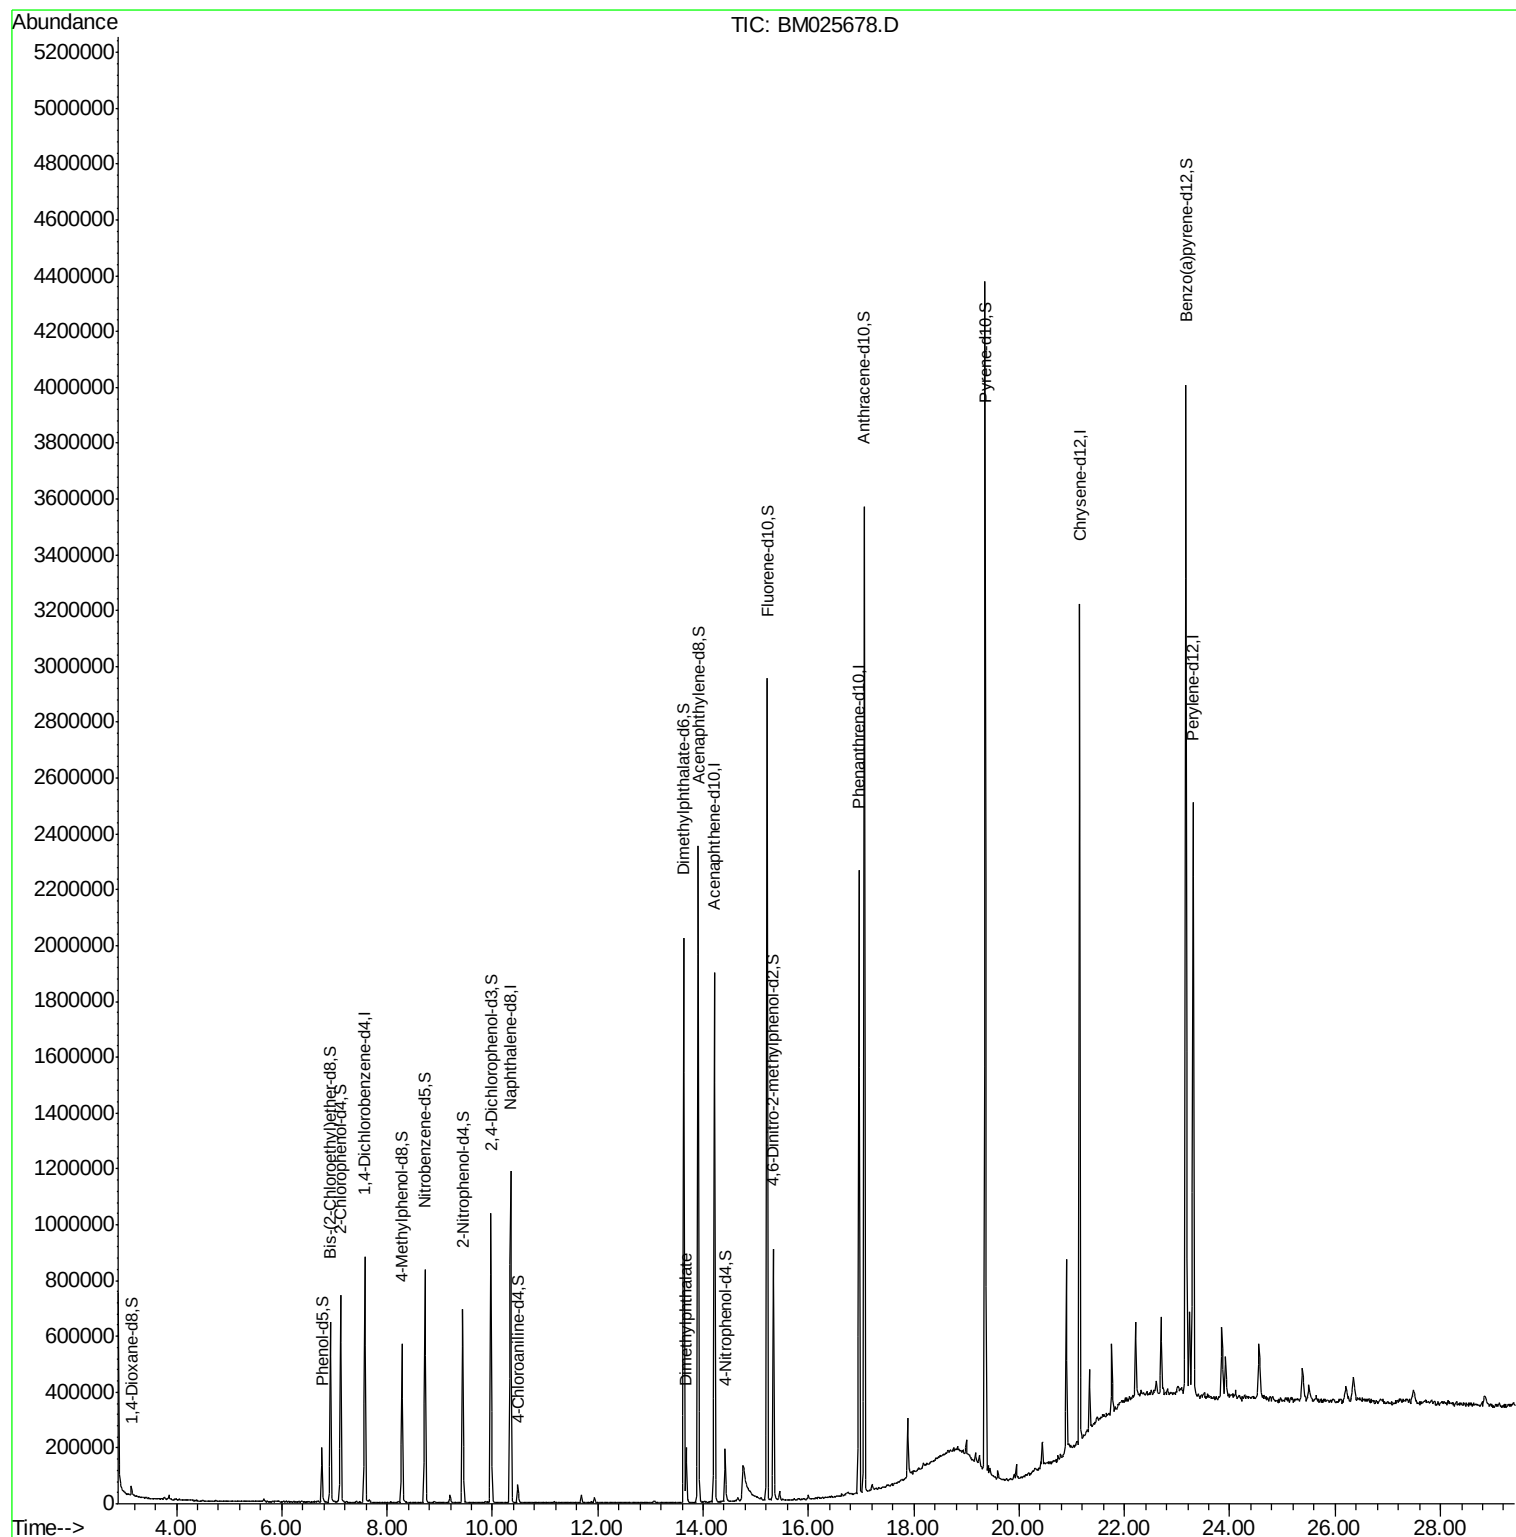

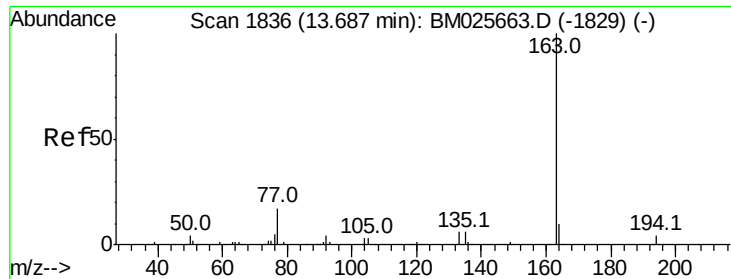

#45

Dimethylphthalate

Concen: 2.386 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BM025678.D

Acq: 21 Mar 2020 01:33

Instrument :

BNA_M

ClientSampleId :

C0DJ6

Tot Ion:163 Resp: 117099

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.3 8.2 12.4

