

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025684.D
 Acq On : 21 Mar 2020 05:46
 Operator : CG/JU
 Sample : L1977-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0A10

Quant Time: Mar 22 07:22:28 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 11:44:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	229352	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	955678	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	591181	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1235891	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1257899	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1399878	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	22137	4.05	ng/uL	0.00
5) Phenol-d5	6.76	99	438733	24.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	253786	24.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	372091	25.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	371375	24.97	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	186783	26.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	207794	27.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	376439	24.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	524454	29.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1118144	24.89	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1385191	25.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	180974	21.16	ng/ul	0.00
58) Fluorene-d10	15.21	176	989710	25.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	133725	17.73	ng/ul	0.00
71) Anthracene-d10	17.06	188	1468862	25.45	ng/ul	0.00
79) Pyrene-d10	19.36	212	1562950	25.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1877679	26.20	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	88961	1.902	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025684.D
Acq On : 21 Mar 2020 05:46
Operator : CG/JU
Sample : L1977-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0A10

Quant Time: Mar 22 07:22:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 11:44:27 2020
Response via : Initial Calibration

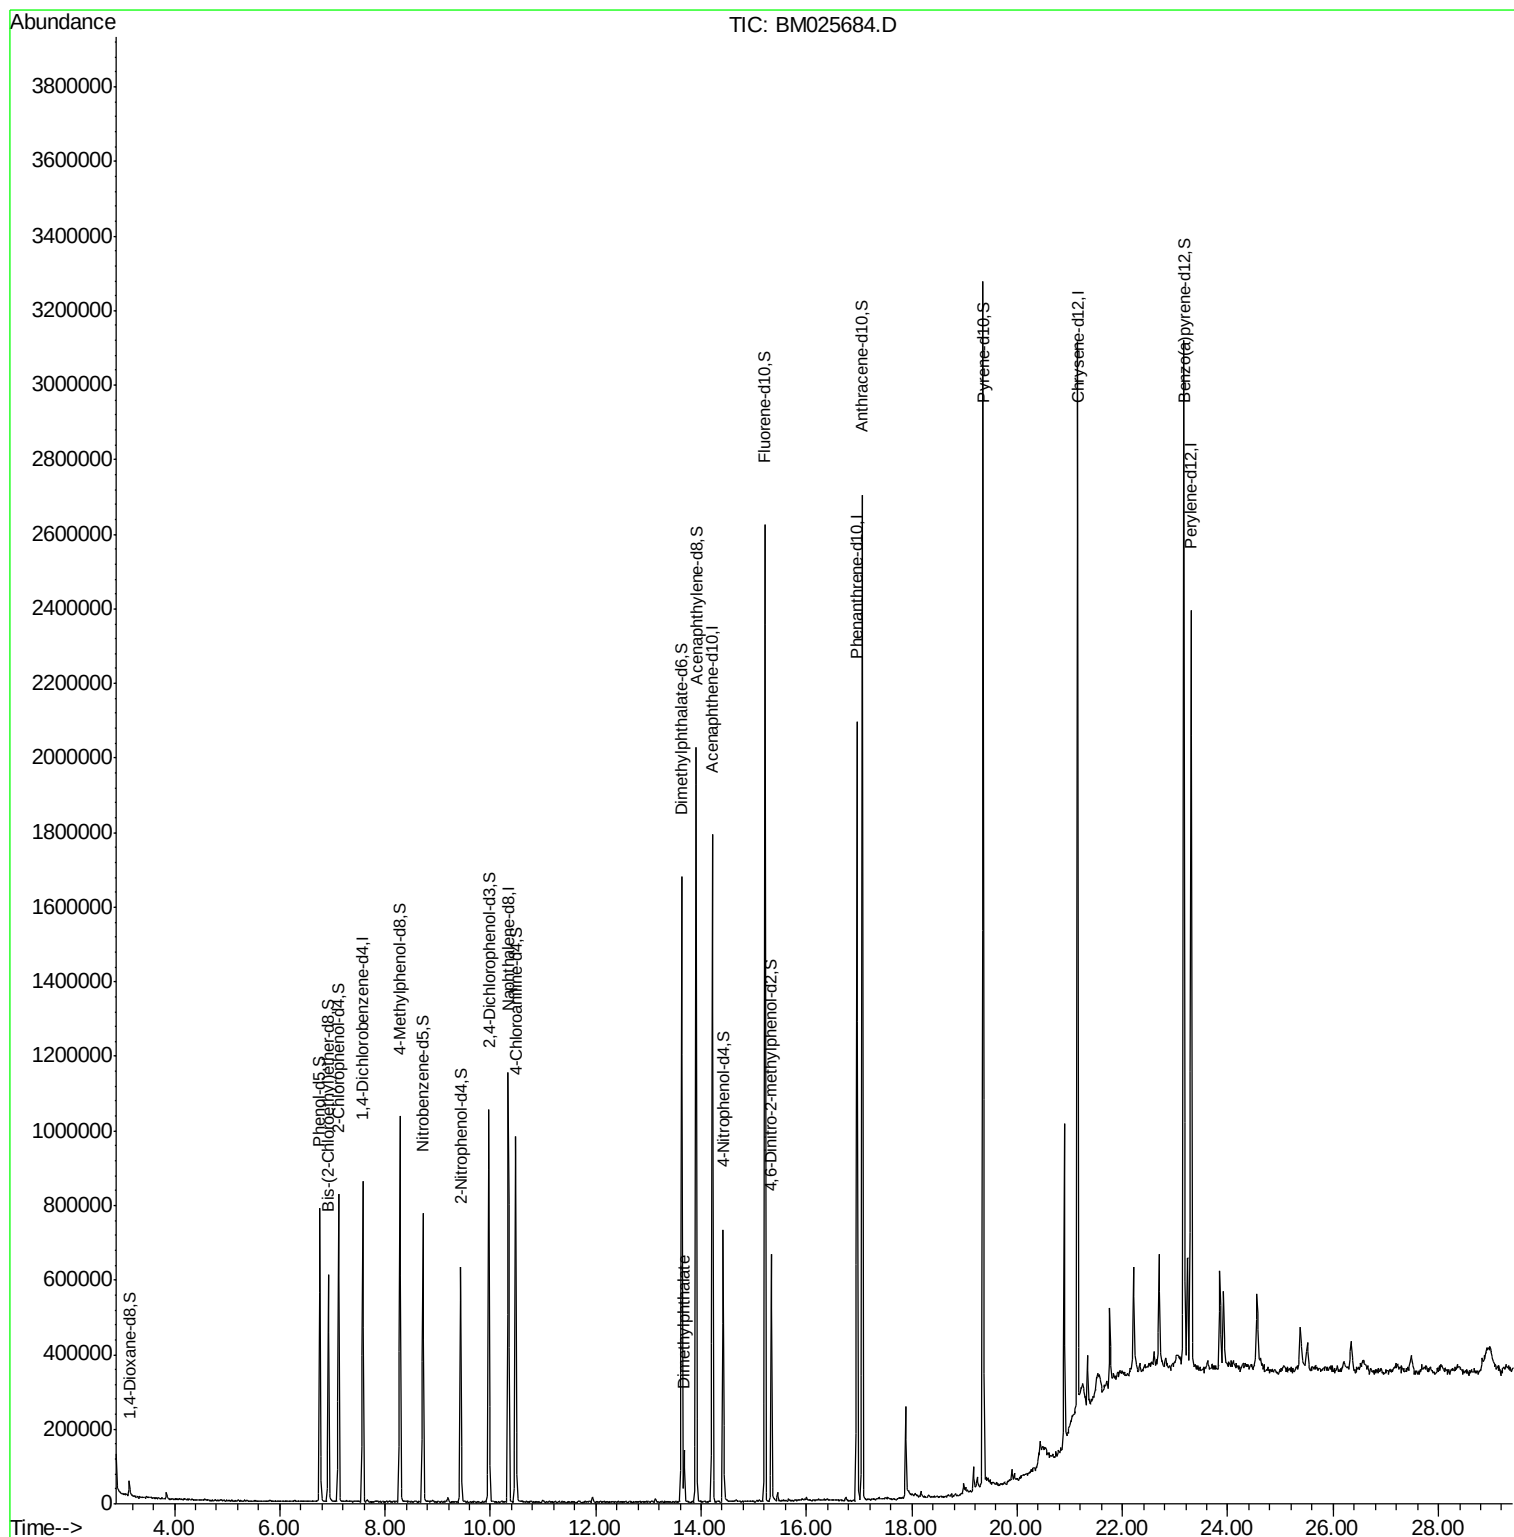

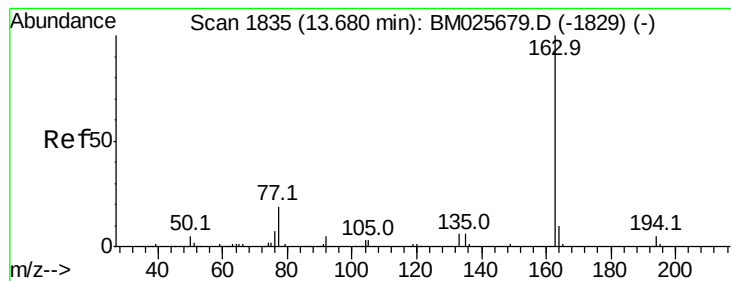

#45

Dimethylphthalate

Concen: 1.902 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. 0.00 min

Lab File: BM025684.D

Acq: 21 Mar 2020 05:46

Instrument :

BNA_M

ClientSampleId :

B0A10


Tot Ion:163 Resp: 88961

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.7 8.2 12.4

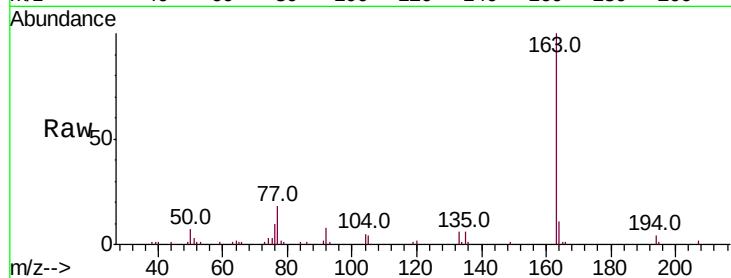

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

