

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025686.D
 Acq On : 21 Mar 2020 06:58
 Operator : CG/JU
 Sample : L1977-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0AH8

Quant Time: Mar 22 07:34:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 11:44:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	229826	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	948316	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	582774	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1210557	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1260211	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1352613	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	21438	3.91	ng/uL	0.00
5) Phenol-d5	6.76	99	433046	23.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	254958	24.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	367378	24.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	355626	23.86	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	186167	26.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	199882	26.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	370460	24.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	483346	27.16	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1092637	24.67	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1373140	25.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	172774	20.49	ng/ul	0.00
58) Fluorene-d10	15.21	176	983960	25.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	126264	17.10	ng/ul	0.00
71) Anthracene-d10	17.06	188	1450607	25.66	ng/ul	0.00
79) Pyrene-d10	19.36	212	1559729	25.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1826299	26.37	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.68	163	96707	2.098	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025686.D
Acq On : 21 Mar 2020 06:58
Operator : CG/JU
Sample : L1977-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0AH8

Quant Time: Mar 22 07:34:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 11:44:27 2020
Response via : Initial Calibration

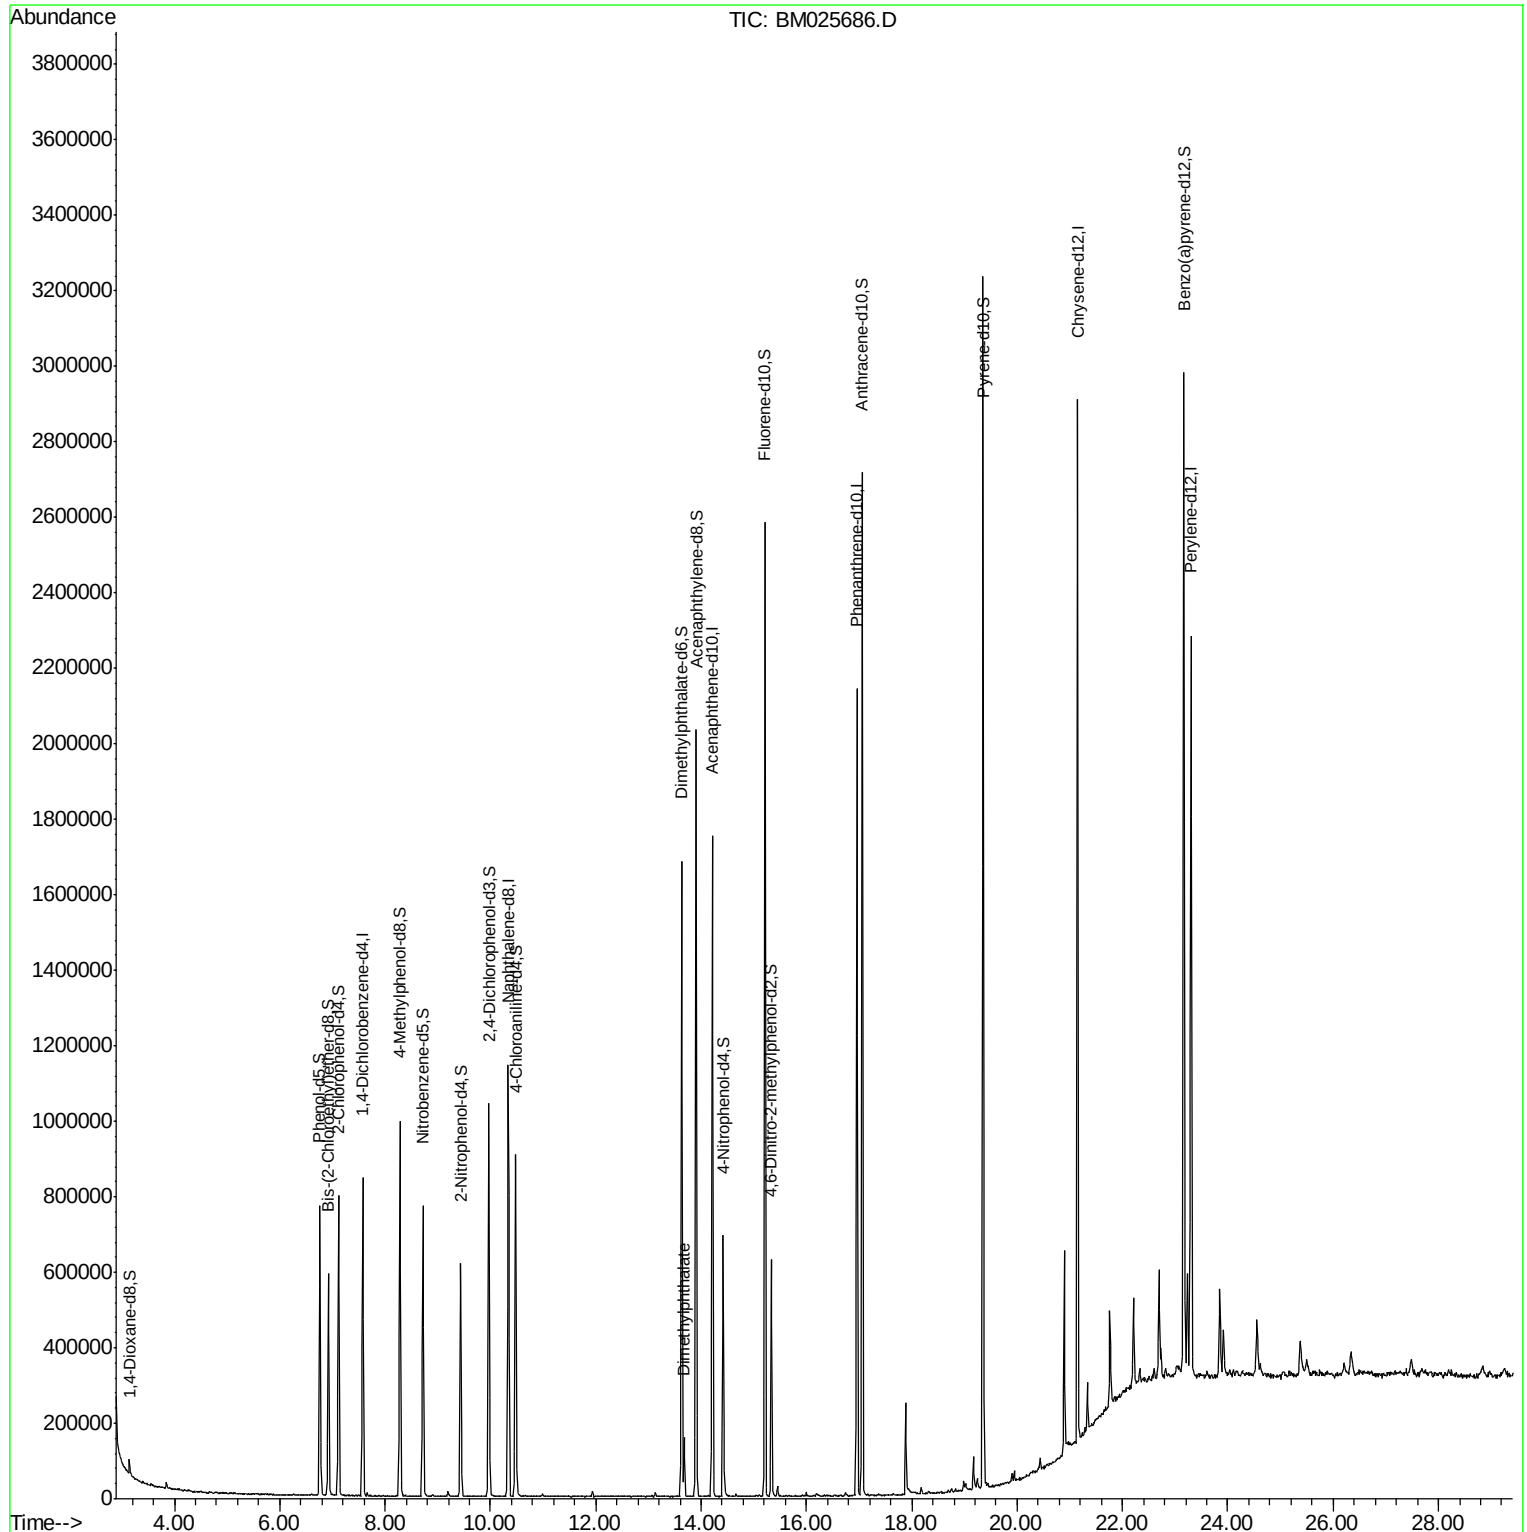

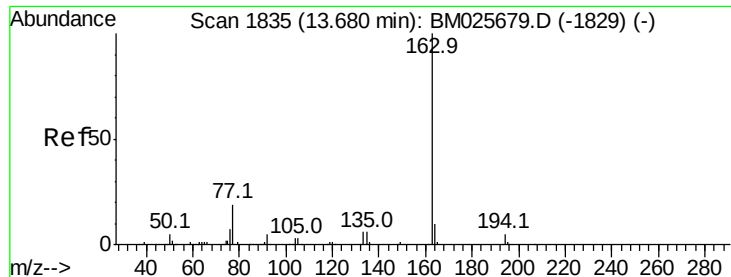

#45

Dimethylphthalate

Concen: 2.098 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BM025686.D

Acq: 21 Mar 2020 06:58

Instrument :

BNA_M

ClientSampleId :

B0AH8


Tot Ion:163 Resp: 96707

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 10.8 8.2 12.4

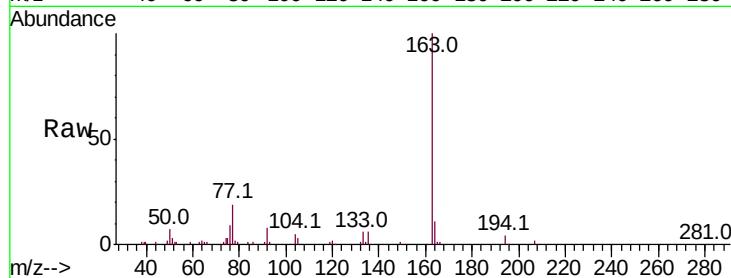

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

