

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025688.D
 Acq On : 21 Mar 2020 08:10
 Operator : CG/JU
 Sample : L1986-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF6T0

Quant Time: Mar 22 07:40:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 11:44:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	209499	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	876607	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	549539	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1171639	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1234309	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1366267	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	25789	5.16	ng/uL	0.00
5) Phenol-d5	6.76	99	476758	28.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	272448	28.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	404393	30.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	396575	29.19	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	198121	30.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	217979	31.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	406886	28.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	534528	32.50	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1197388	28.67	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1498610	29.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	187052	23.52	ng/ul	0.00
58) Fluorene-d10	15.21	176	1062244	28.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	143090	20.02	ng/ul	0.00
71) Anthracene-d10	17.06	188	1579951	28.87	ng/ul	0.00
79) Pyrene-d10	19.36	212	1697969	28.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2055326	29.38	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	355253	8.171	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025688.D
Acq On : 21 Mar 2020 08:10
Operator : CG/JU
Sample : L1986-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF6T0

Quant Time: Mar 22 07:40:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 11:44:27 2020
Response via : Initial Calibration

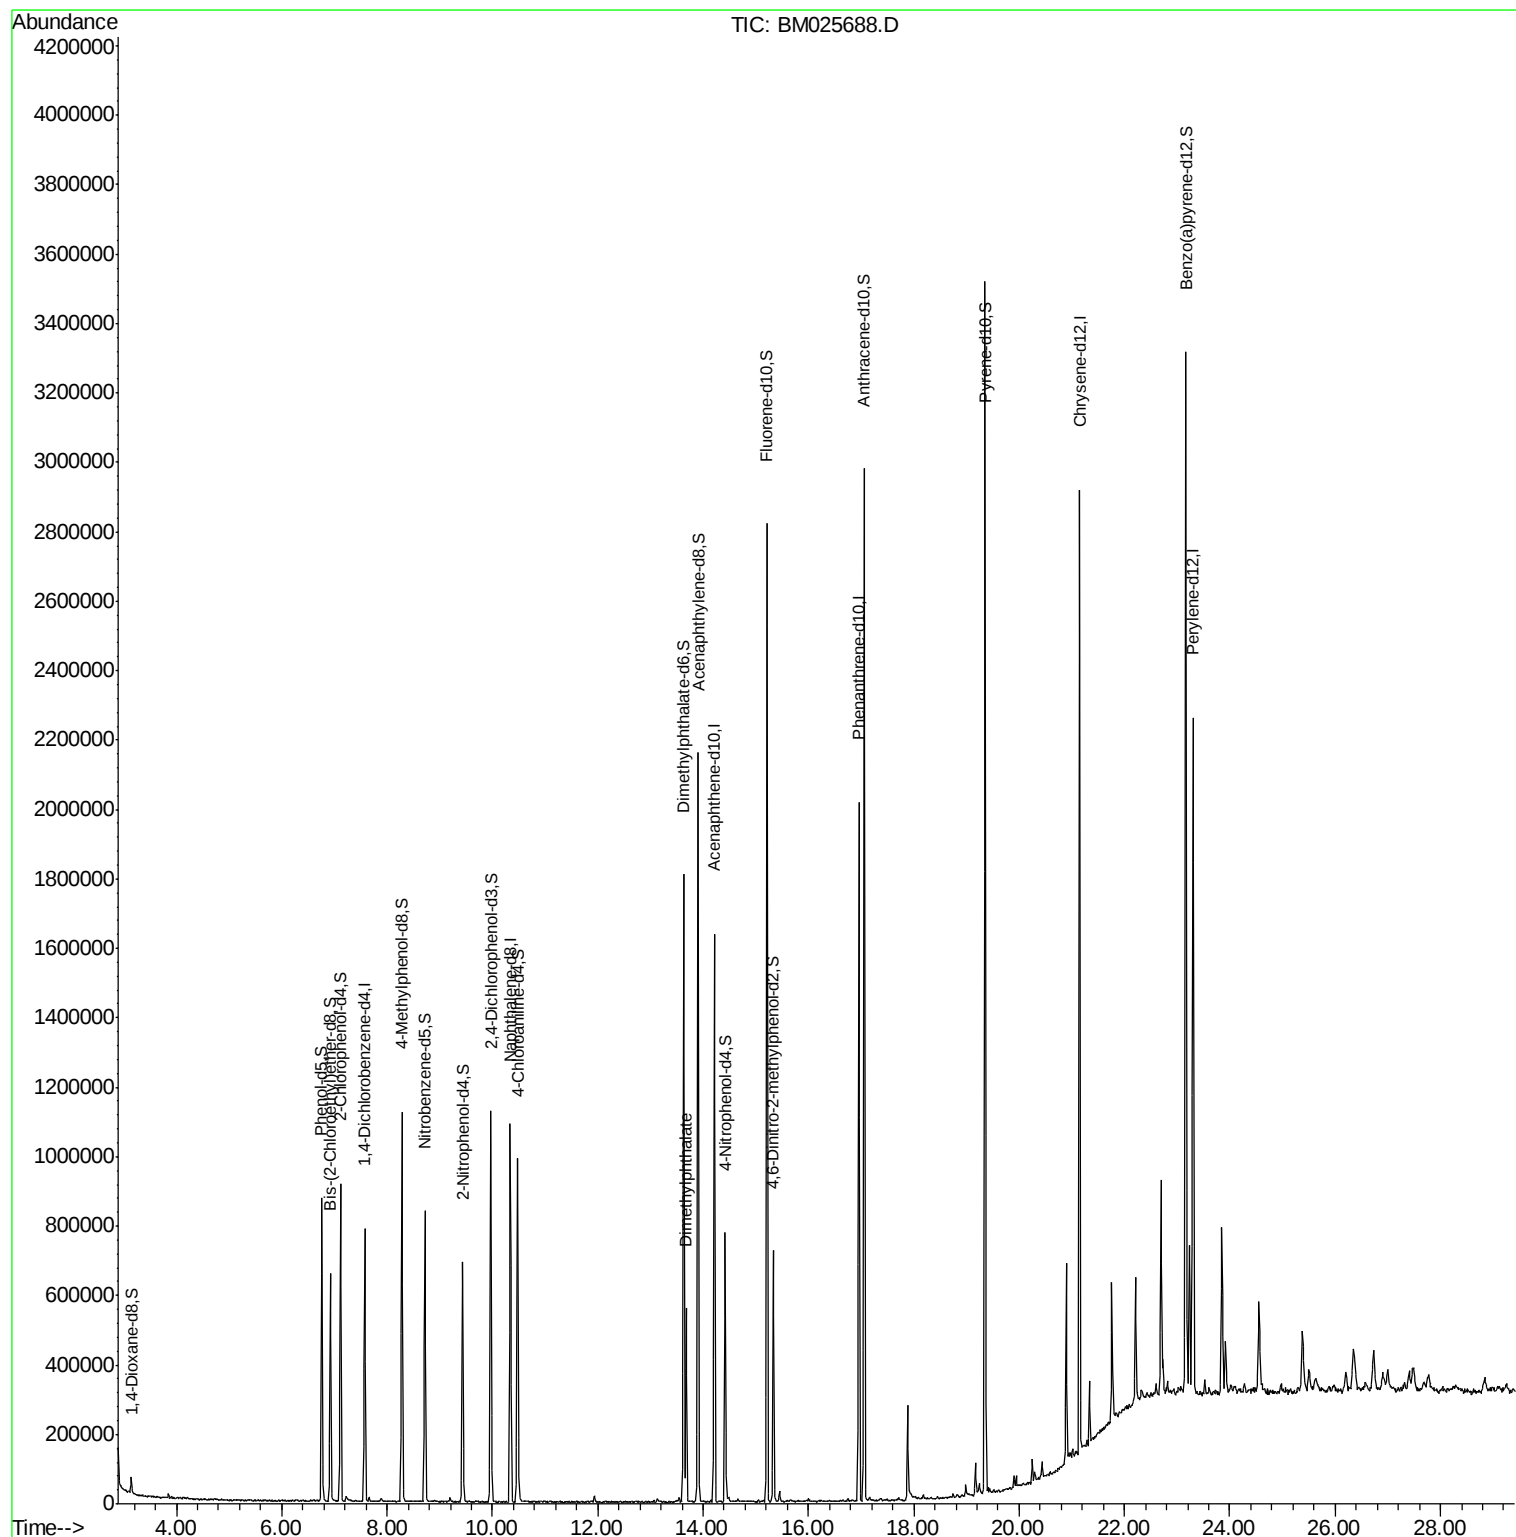

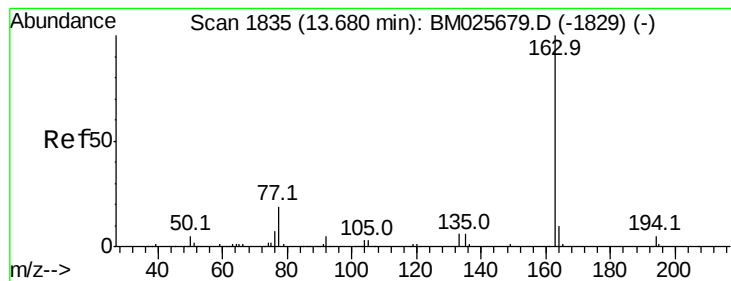

#45

Dimethylphthalate

Concen: 8.171 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BM025688.D

Acq: 21 Mar 2020 08:10

Instrument :

BNA_M

ClientSampleId :

BF6T0


Tot Ion:163 Resp: 355253

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.0 8.2 12.4

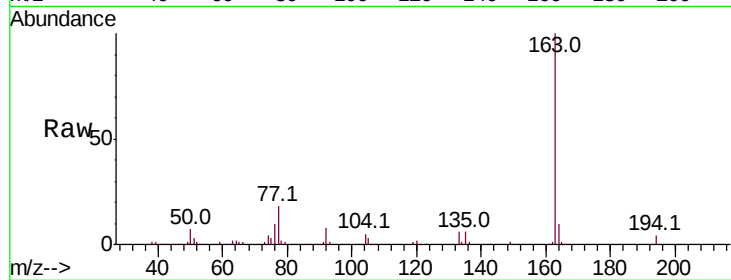

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

