

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
 Data File : BM025689.D
 Acq On : 21 Mar 2020 08:46
 Operator : CG/JU
 Sample : L1986-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF6T2

Quant Time: Mar 22 07:43:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 20 11:44:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	188201	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	780660	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	484912	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1028426	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1066704	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1172528	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	23063	5.14	ng/uL	0.00
5) Phenol-d5	6.76	99	412020	27.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	239973	28.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	350911	29.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	341836	28.01	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	172659	29.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	187656	30.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	353227	28.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	454907	31.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1019083	27.65	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1274332	28.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	155040	22.10	ng/ul	0.00
58) Fluorene-d10	15.21	176	905552	27.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	118658	18.91	ng/ul	0.00
71) Anthracene-d10	17.06	188	1350595	28.12	ng/ul	0.00
79) Pyrene-d10	19.36	212	1434296	27.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1716066	28.59	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.68	163	84580	2.205	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032020\
Data File : BM025689.D
Acq On : 21 Mar 2020 08:46
Operator : CG/JU
Sample : L1986-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF6T2

Quant Time: Mar 22 07:43:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 20 11:44:27 2020
Response via : Initial Calibration

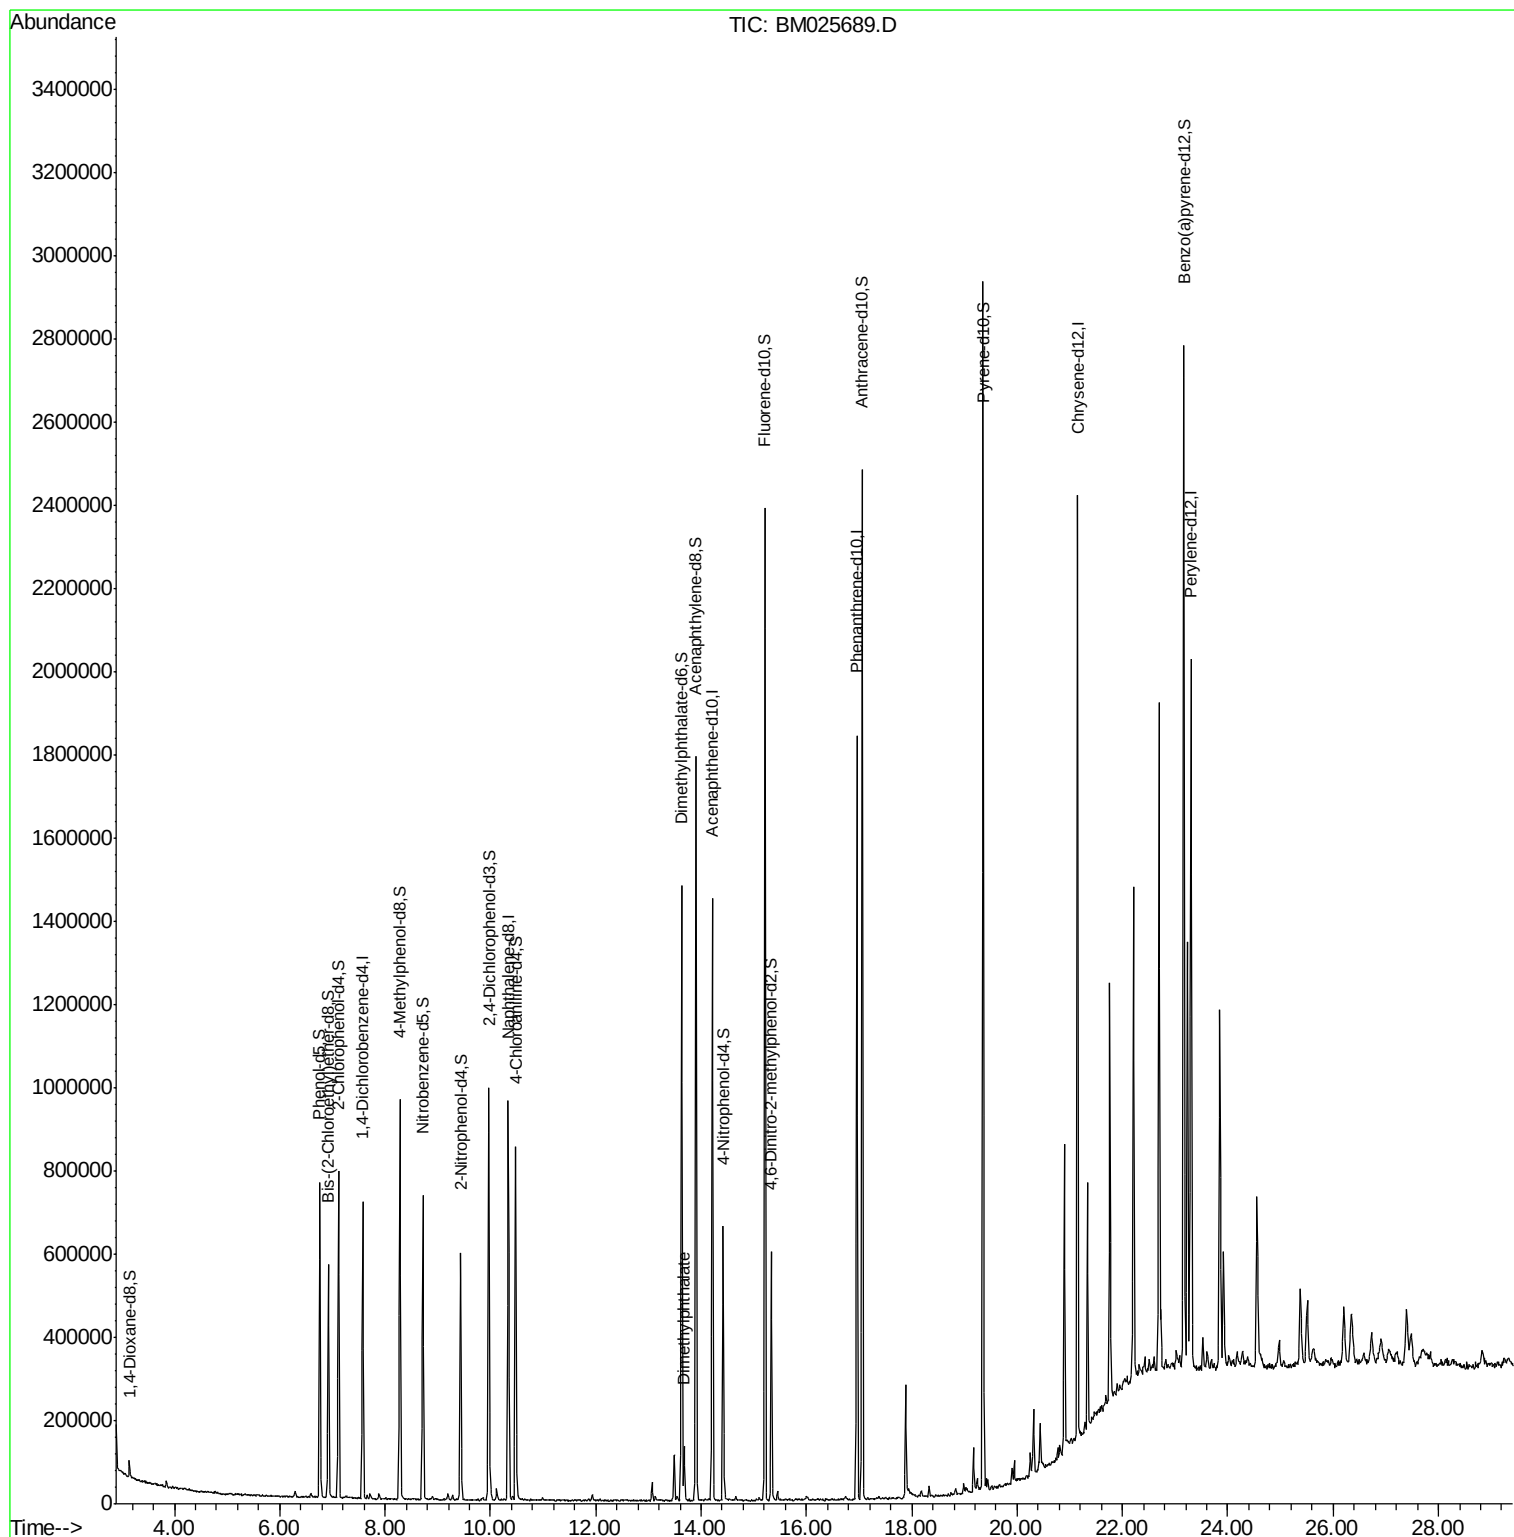

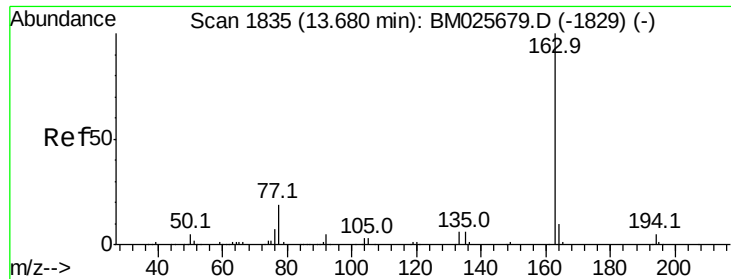

#45

Dimethylphthalate

Concen: 2.205 ng/ul

RT: 13.68 min Scan# 1835

Delta R.T. -0.00 min

Lab File: BM025689.D

Acq: 21 Mar 2020 08:46

Instrument :

BNA_M

ClientSampleId :

BF6T2

Tot Ion:163 Resp: 84580

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 9.7 8.2 12.4

