
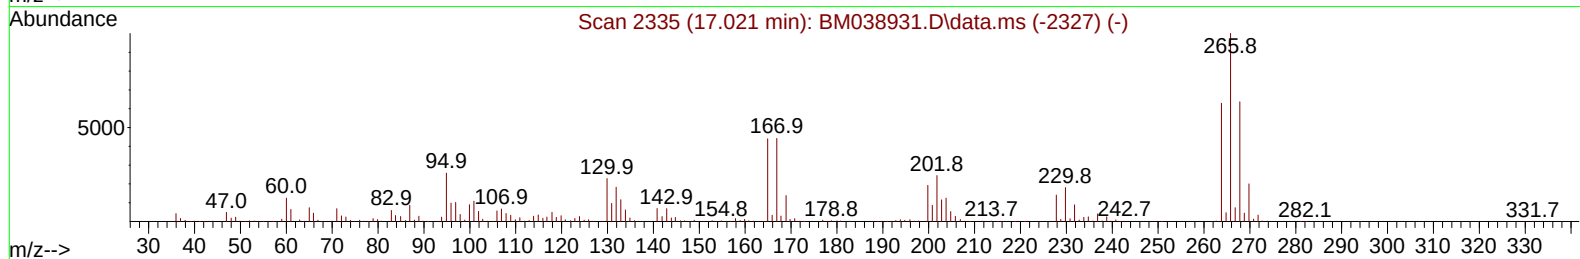
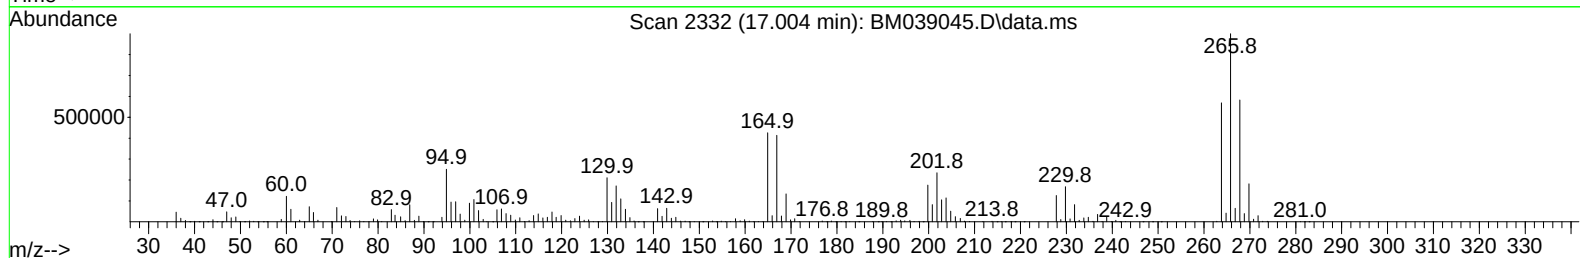


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
Data File : BM039045.D
Acq On : 20 Mar 2023 15:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 08:31:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 05:25:34 2023
Response via : Initial Calibration

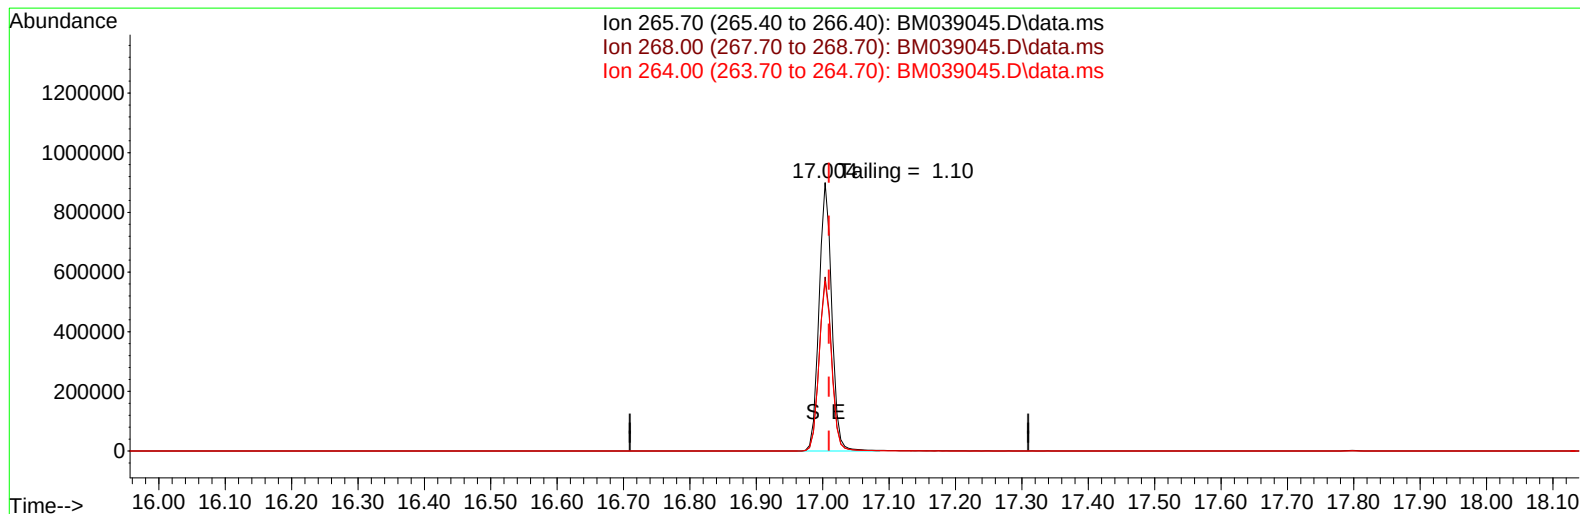

TIC: BM039045.D\data.ms

(70) Pentachlorophenol (C)




17.004min (-0.006) 561518.79 ng

response 1196821

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.81
264.00	62.90	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
Data File : BM039045.D
Acq On : 20 Mar 2023 15:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 08:31:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 05:25:34 2023
Response via : Initial Calibration

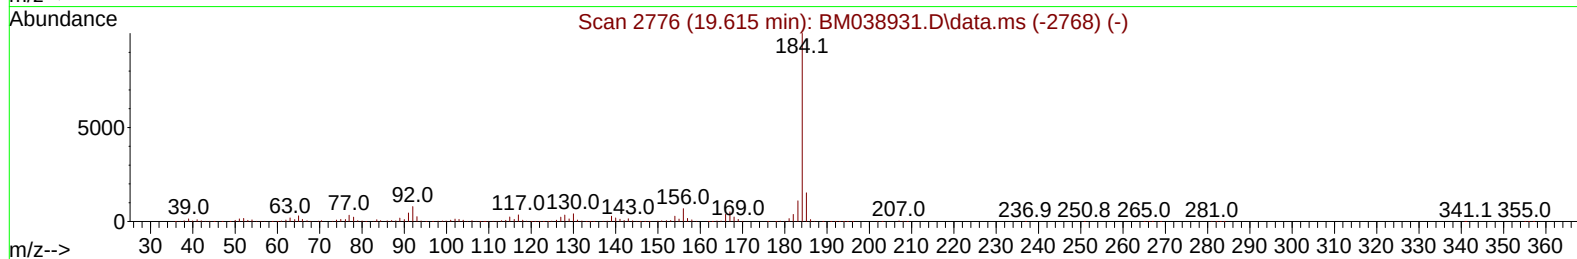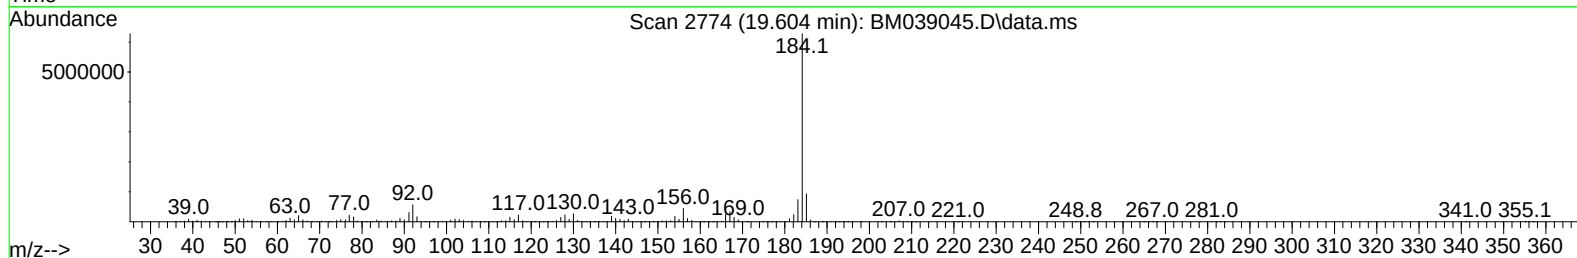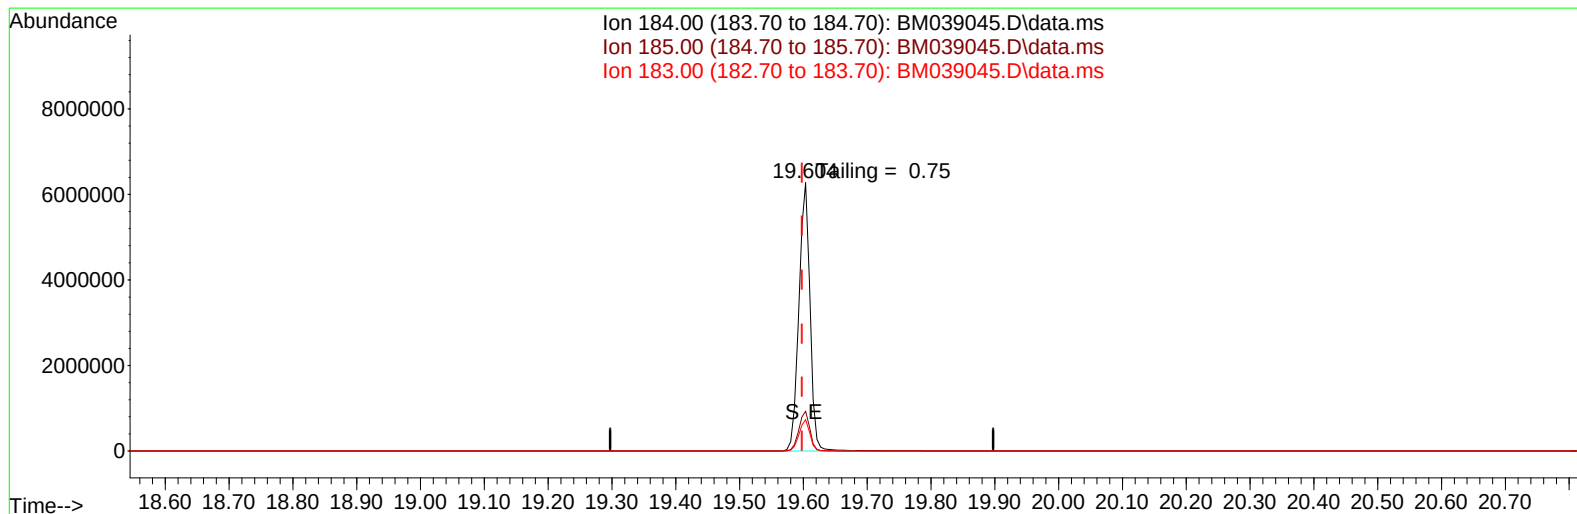

TIC: BM039045.D\data.ms

(77) Benzidine

19.604min (+ 0.006) 2361913.35 ng

response 7610587

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.84
183.00	11.00	11.71
0.00	0.00	0.00