
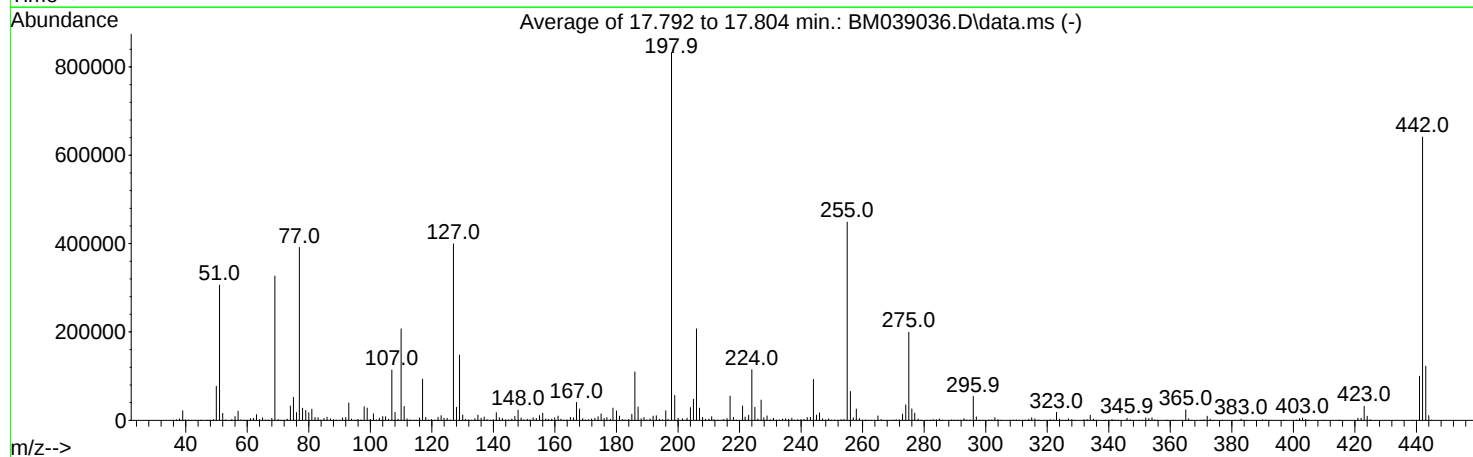


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
 Data File : BM039036.D
 Acq On : 20 Mar 2023 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 05:25:34 2023

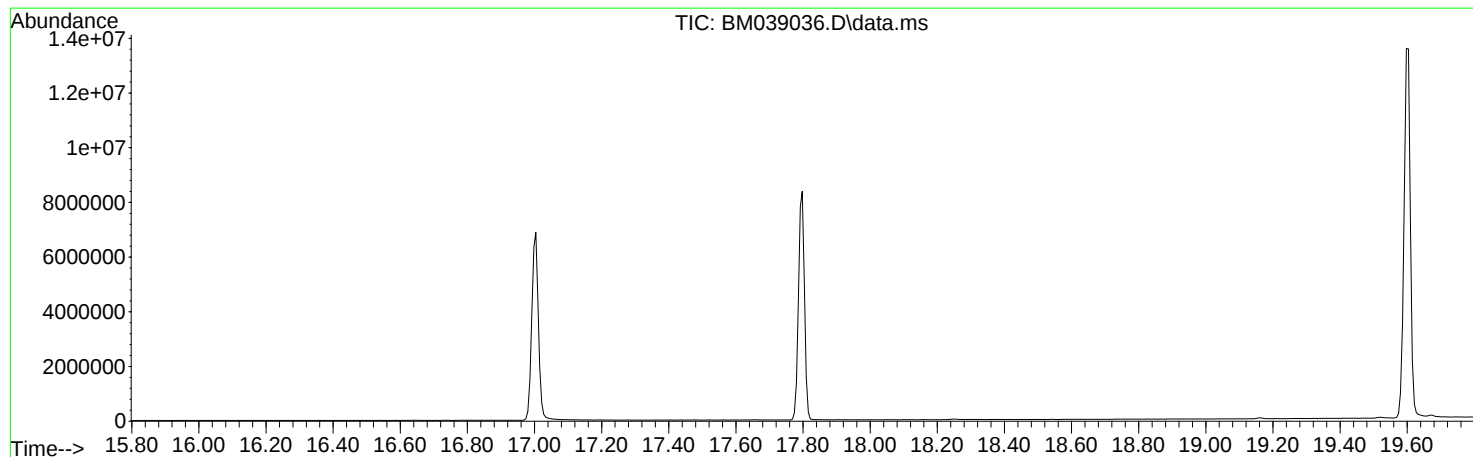




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	306143	PASS
68	69	0.00	2	1.4	4731	PASS
69	198	0.00	100	39.2	326773	PASS
70	69	0.00	2	0.5	1773	PASS
127	198	10	80	47.9	399381	PASS
197	198	0.00	2	0.2	1990	PASS
198	198	100	100	100.0	832917	PASS
199	198	5	9	6.8	56344	PASS
275	198	10	60	23.9	199403	PASS
365	198	1	100	2.9	23928	PASS
441	198	0.01	100	12.0	100016	PASS
442	442	50	100	100.0	641301	PASS
443	442	15	24	19.1	122763	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
 Data File : BM039036.D
 Acq On : 20 Mar 2023 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 20 17:28:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 05:25:34 2023
 Response via : Initial Calibration

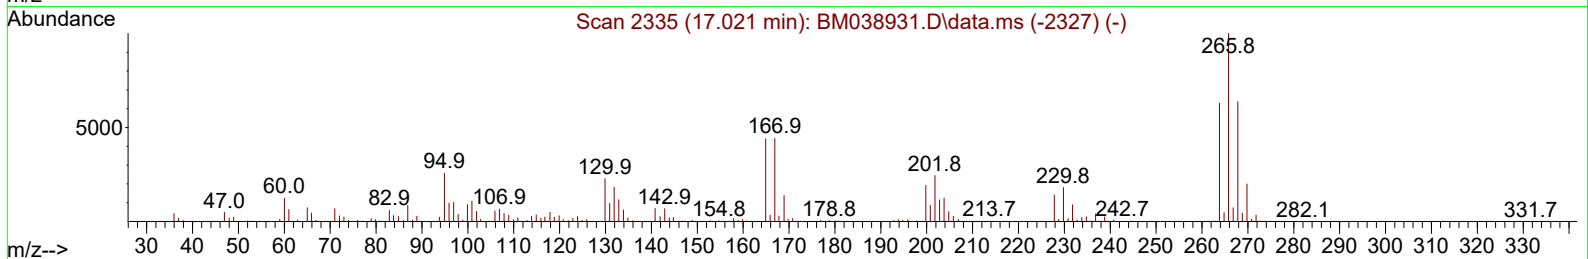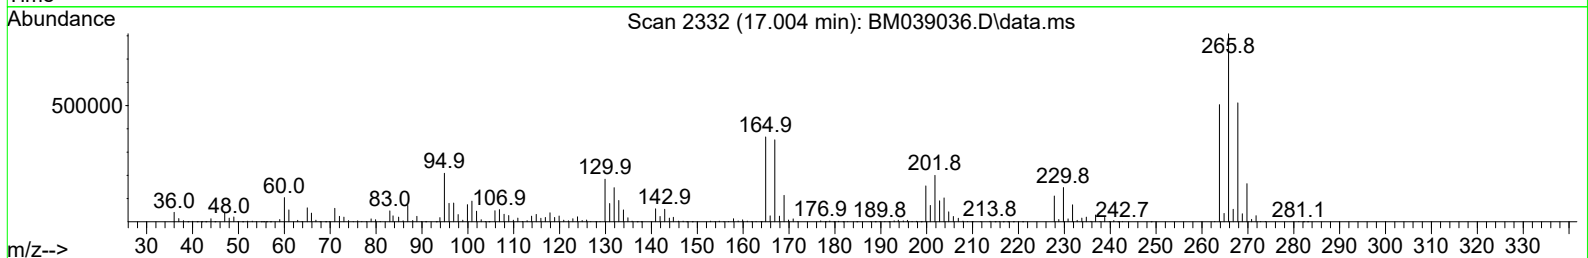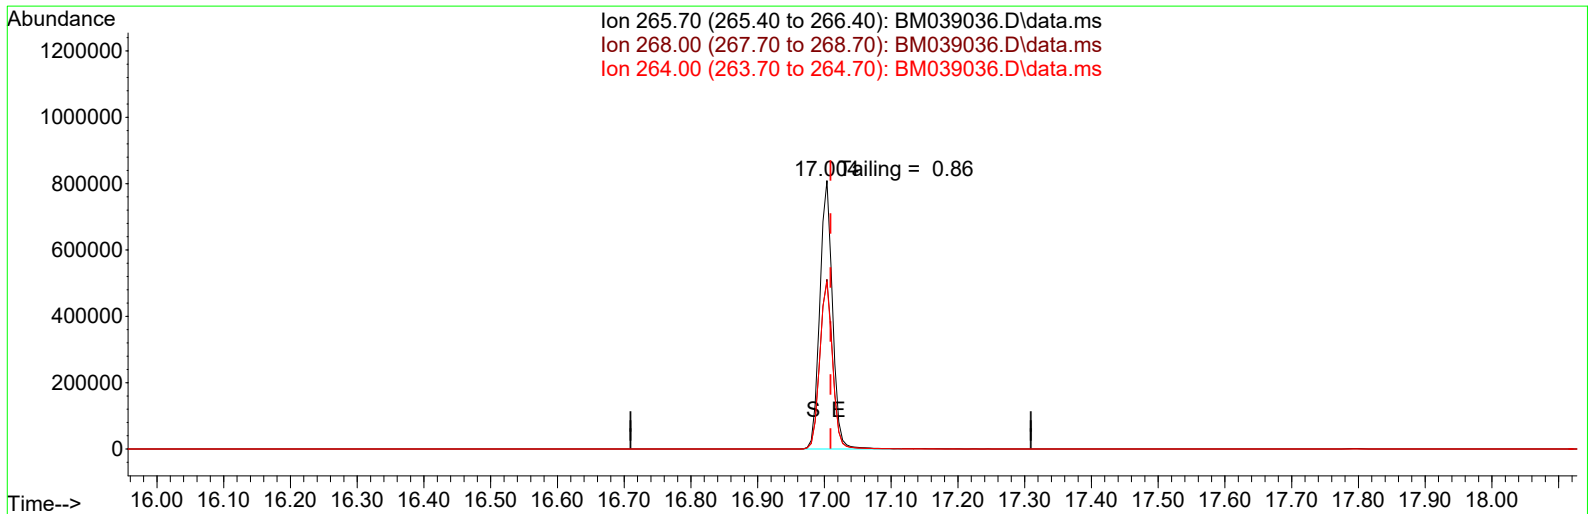

TIC: BM039036.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.006) 0.00 ng




response 1067550

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.22
264.00	62.90	62.27
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\  
Data File : BM039036.D  
Acq On    : 20 Mar 2023  09:43  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 20 17:28:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 05:25:34 2023
Response via : Initial Calibration

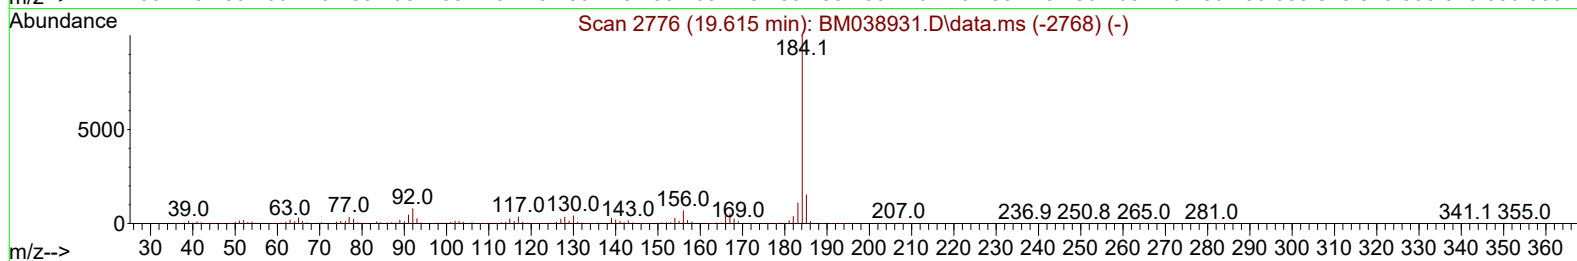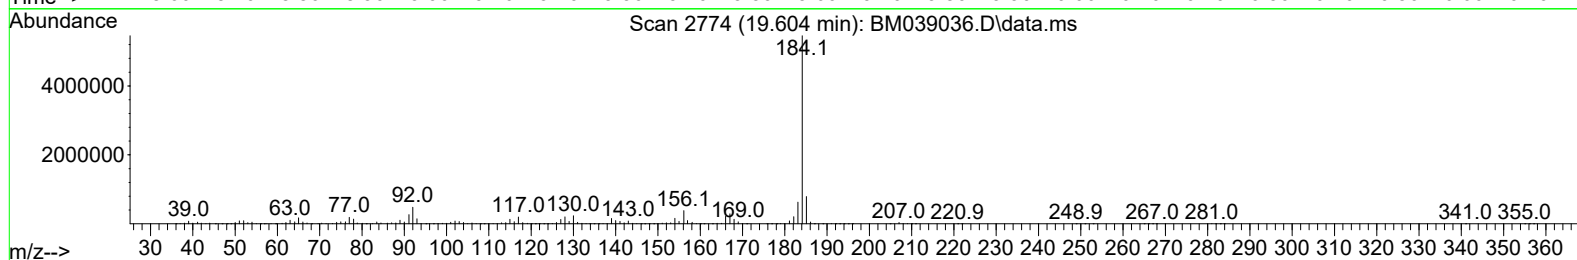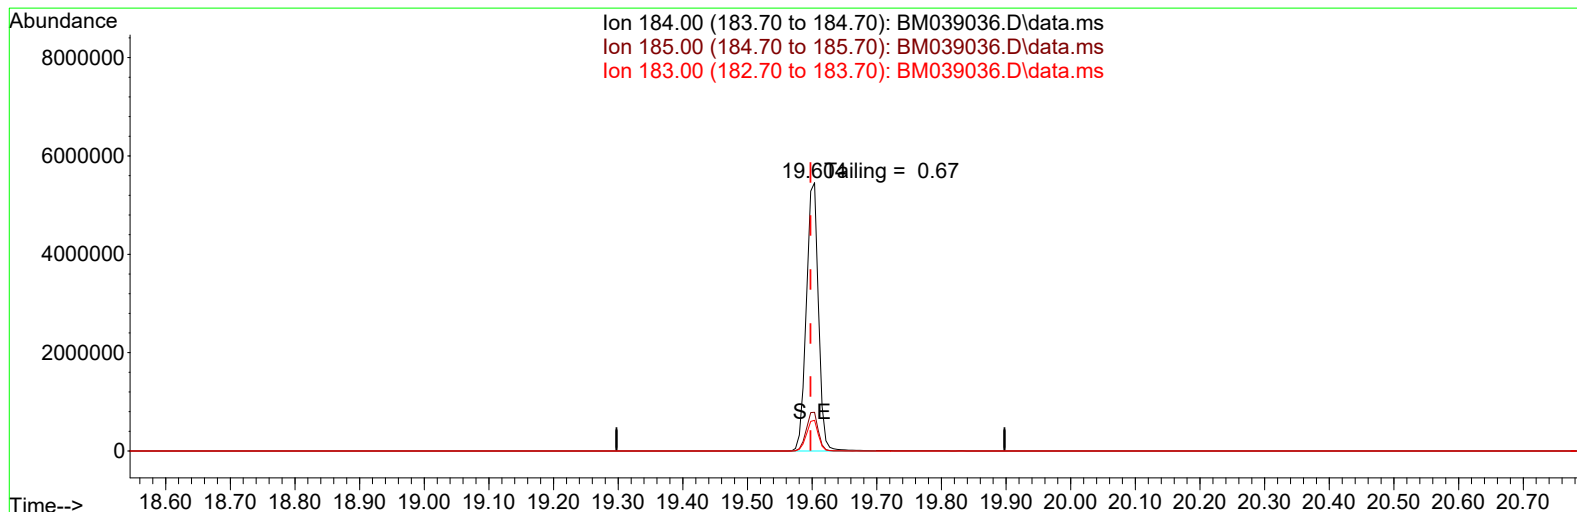

TIC: BM039036.D\data.ms

(77) Benzidine

19.604min (+ 0.006) 3564744.75 ng

response 7145067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.47
183.00	11.00	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/20/2023	BNA_M	<u>BM039036.D</u>
Compound Name	Response	Retention Time
DDT	3011064	20.833
DDD	26136	20.445
DDE	1300	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27436	3038500	0.90

Instrument :
BNA_M
ClientSampleId :
DFTPP