
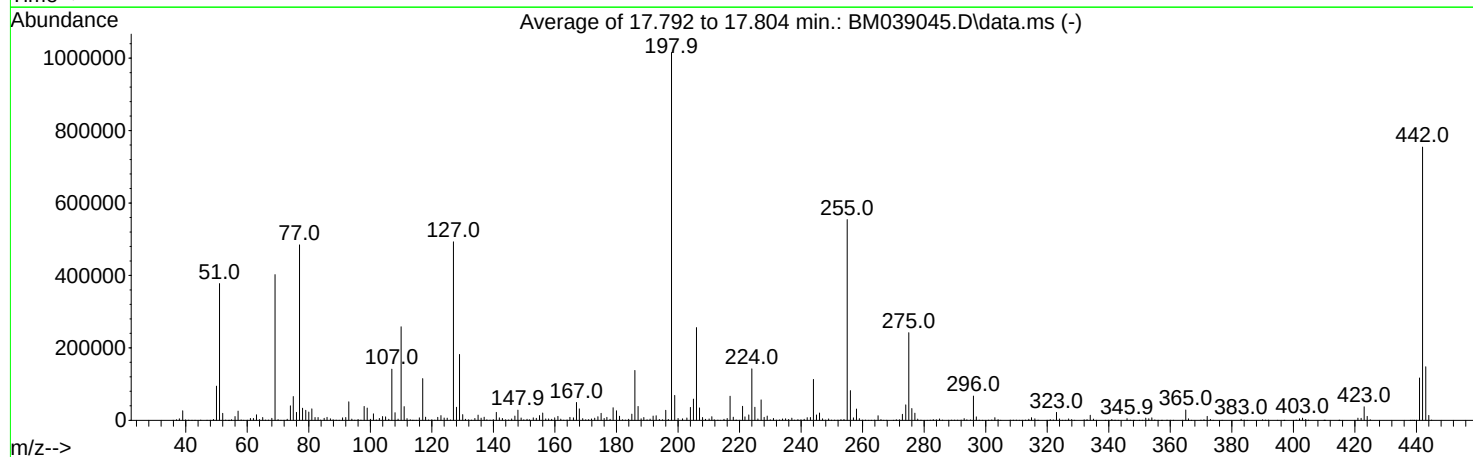


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
 Data File : BM039045.D
 Acq On : 20 Mar 2023 15:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 05:25:34 2023

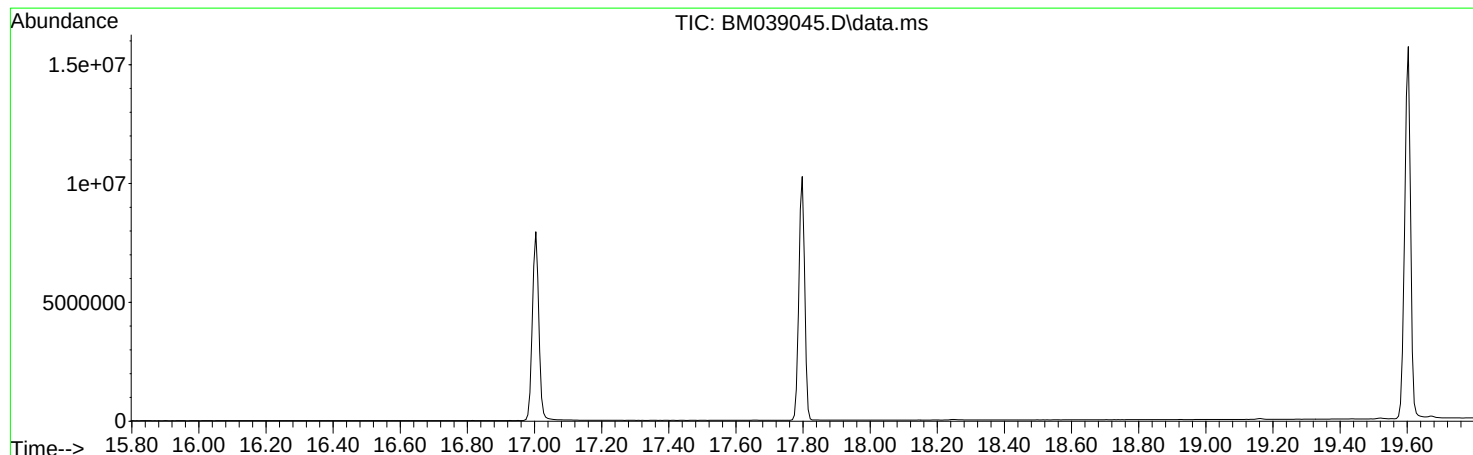




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	377598	PASS
68	69	0.00	2	1.4	5627	PASS
69	198	0.00	100	39.6	402389	PASS
70	69	0.00	2	0.5	1991	PASS
127	198	10	80	48.5	493035	PASS
197	198	0.00	2	0.2	2475	PASS
198	198	100	100	100.0	1015787	PASS
199	198	5	9	6.8	68632	PASS
275	198	10	60	23.8	242069	PASS
365	198	1	100	2.8	28451	PASS
441	198	0.01	100	11.5	116763	PASS
442	442	50	100	100.0	754603	PASS
443	442	15	24	19.6	147821	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
Data File : BM039045.D
Acq On : 20 Mar 2023 15:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 21 08:31:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 05:25:34 2023
Response via : Initial Calibration

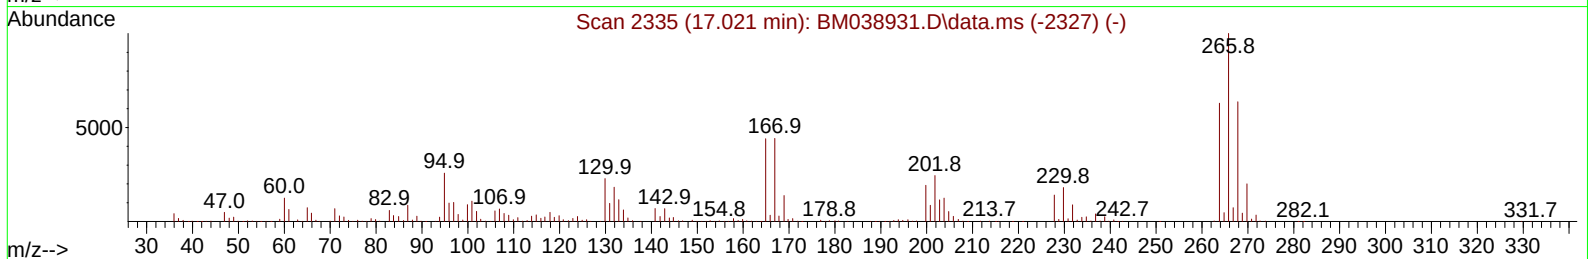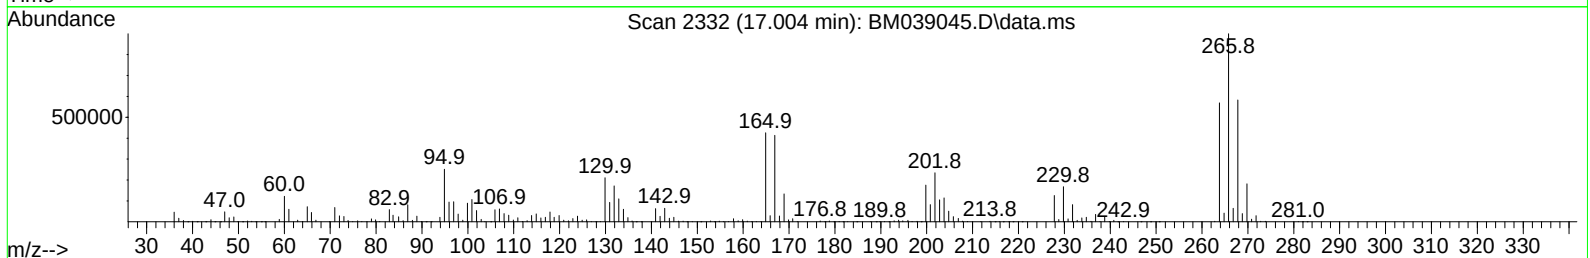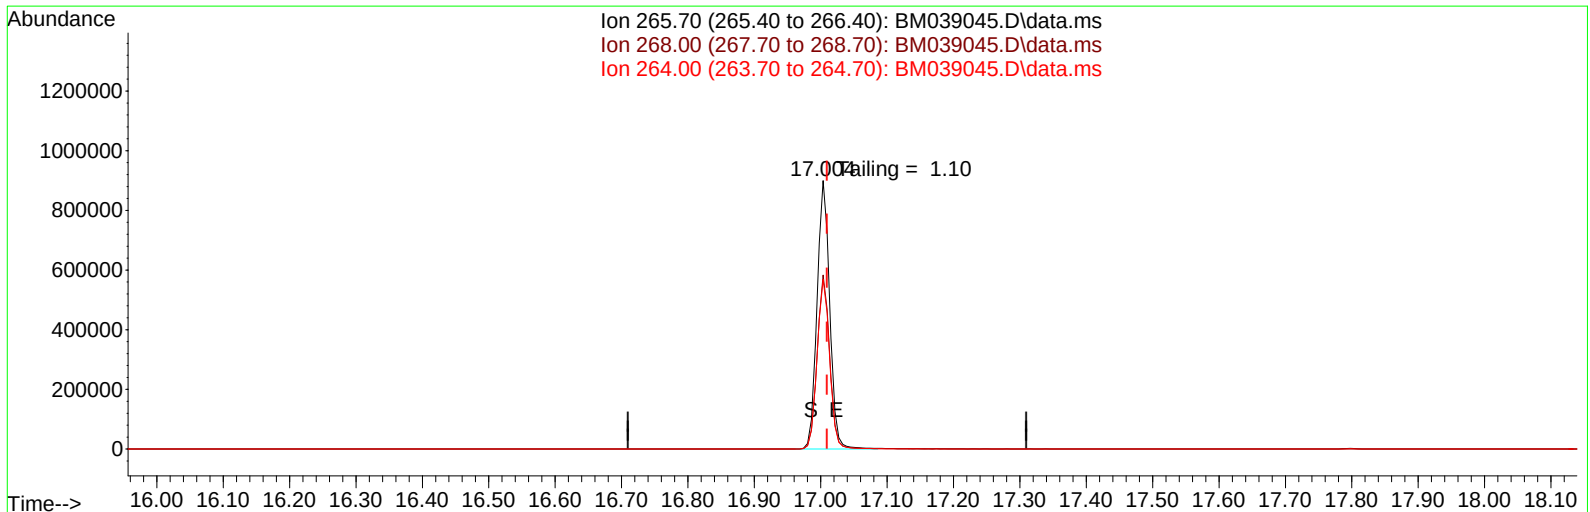

TIC: BM039045.D\data.ms

(70) Pentachlorophenol (C)

17.004min (-0.006) 561518.79 ng




response 1196821

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.81
264.00	62.90	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032023\
 Data File : BM039045.D
 Acq On : 20 Mar 2023 15:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 21 08:31:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 05:25:34 2023
 Response via : Initial Calibration

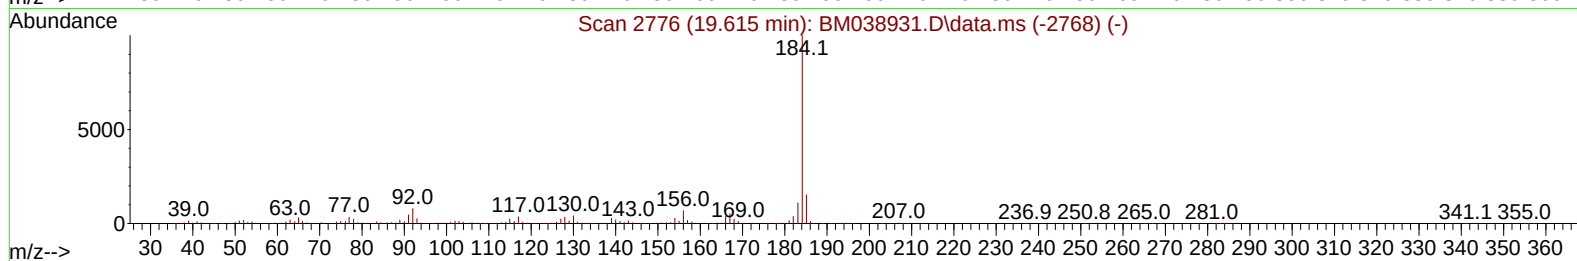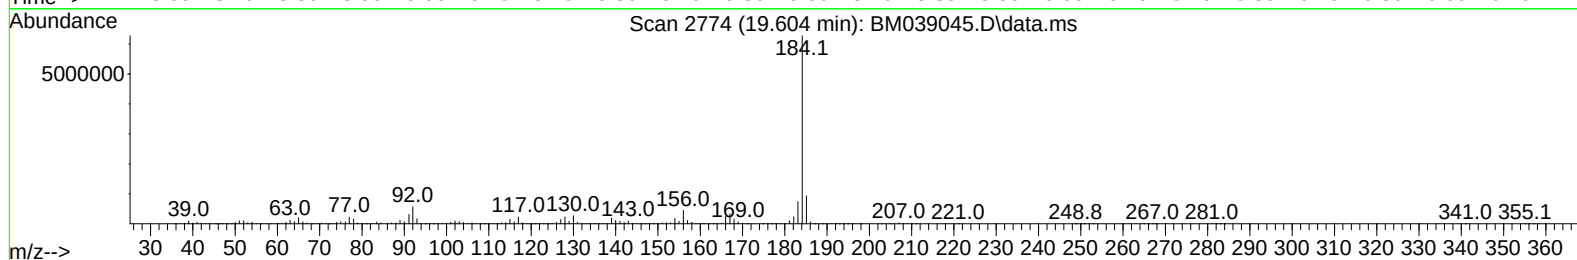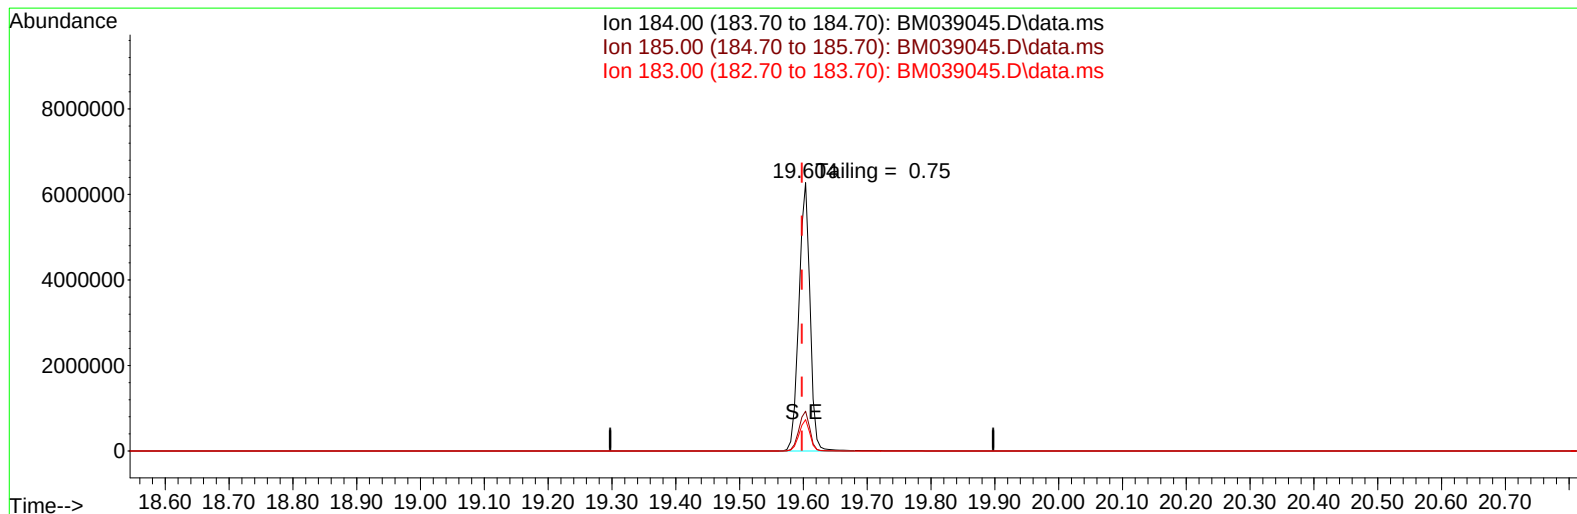

TIC: BM039045.D\data.ms

(77) Benzidine

19.604min (+ 0.006) 2361913.35 ng

response 7610587

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.84
183.00	11.00	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/20/2023	BNA_M	<u>BM039045.D</u>
Compound Name	Response	Retention Time
DDT	3441501	20.833
DDD	29005	20.445
DDE	815	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29820	3471321	0.86

Instrument :
BNA_M
ClientSampleId :
DFTPP