
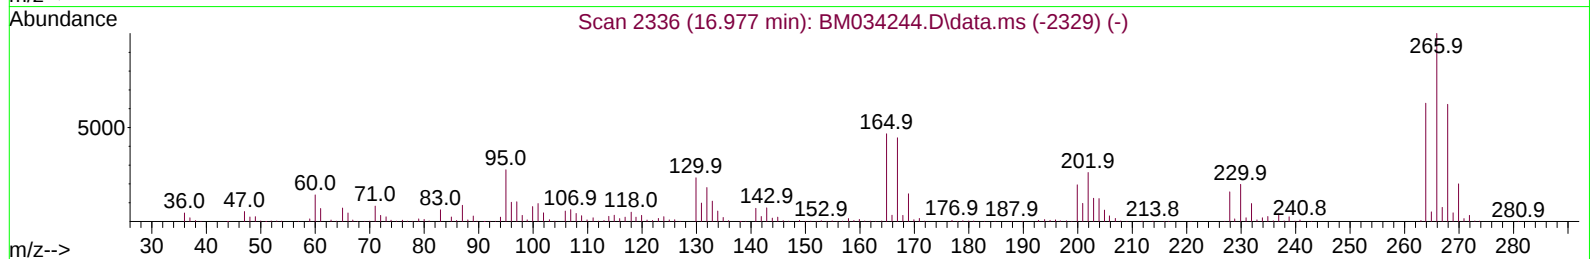
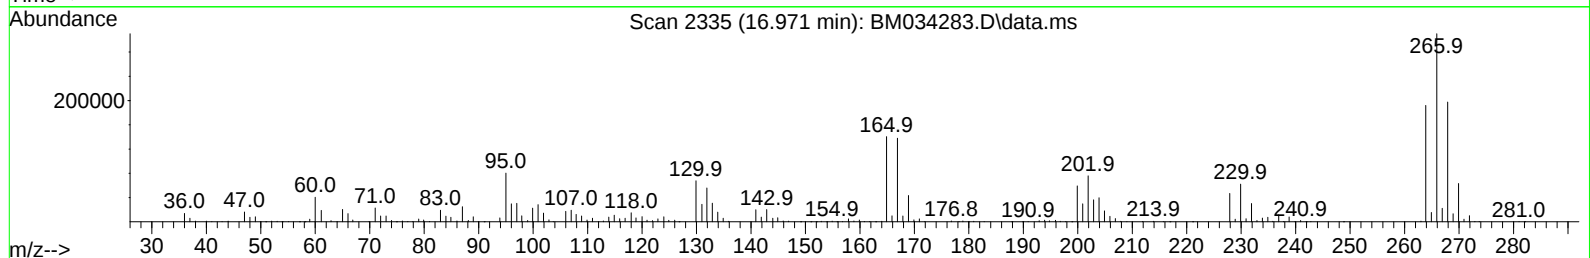


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034283.D
Acq On : 21 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 17:52:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

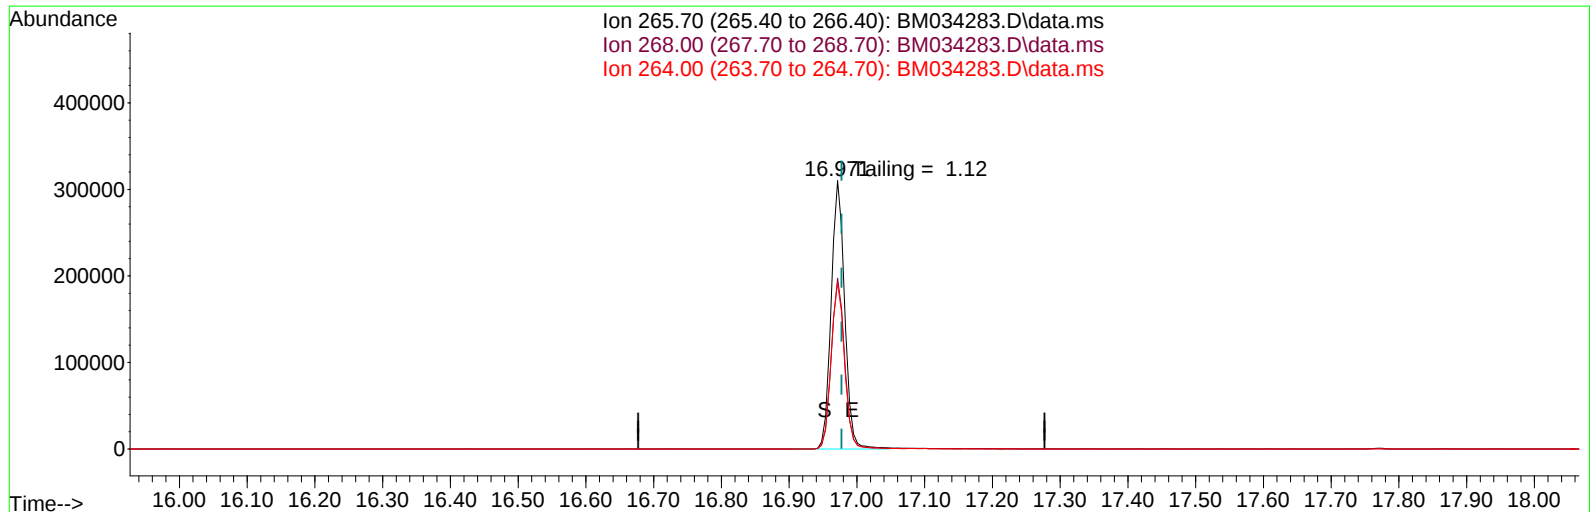

TIC: BM034283.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.006) 175994.66 ng

response 428598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.70
264.00	62.90	61.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034283.D
Acq On : 21 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 17:52:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

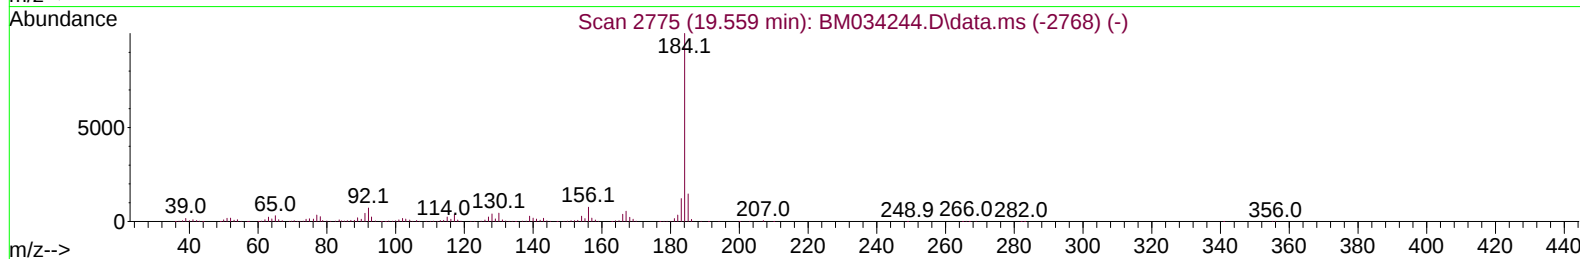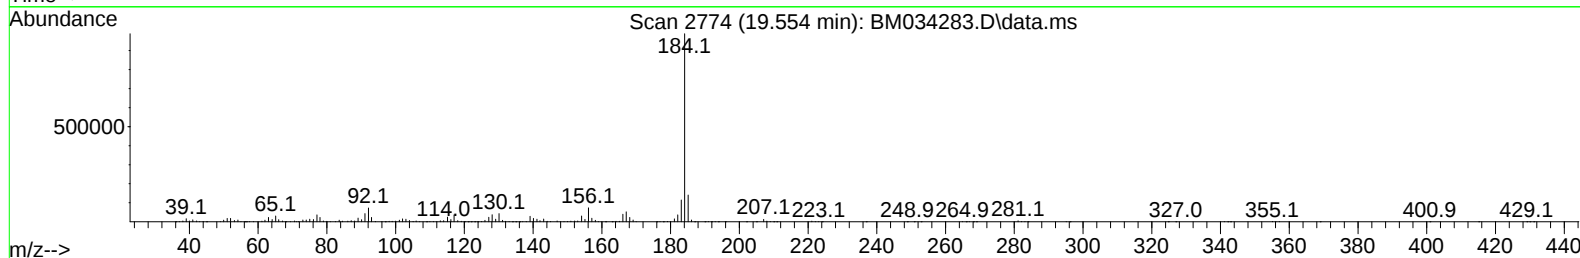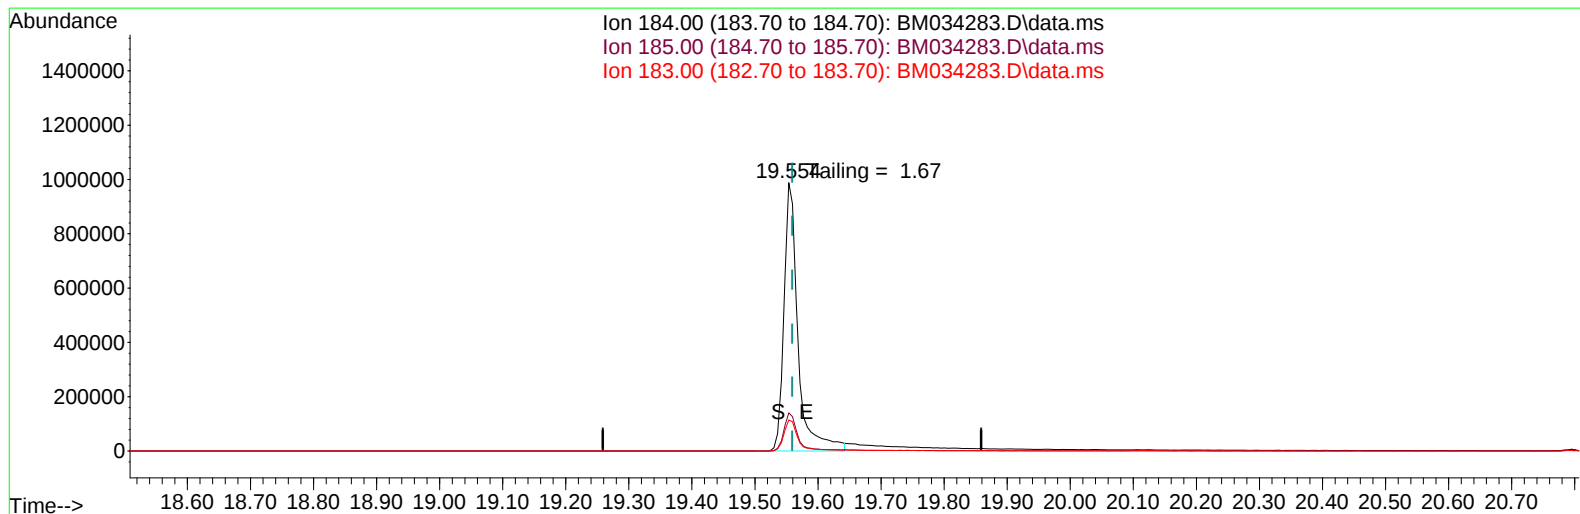

TIC: BM034283.D\data.ms

(77) Benzidine**19.554min (-0.005) 8062.90 ng****response 1694366**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.21
183.00	12.20	11.57
0.00	0.00	0.00