

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034285.D
Acq On : 21 Mar 2022 10:47
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	377	384	395	rBV	4279859	6166038	48.52%	10.830%
2	7.101	649	657	675	rBV	3922546	6272729	49.36%	11.017%
3	7.943	793	800	810	rBV	797054	1272618	10.01%	2.235%
4	9.107	989	998	1018	rBV	2396063	4030007	31.71%	7.078%
5	10.754	1269	1278	1298	rBV	975889	1709837	13.45%	3.003%
6	13.213	1689	1696	1709	rBV	6337534	8992101	70.76%	15.793%
7	14.583	1922	1929	1940	rBV	1517438	2199865	17.31%	3.864%
8	16.066	2174	2181	2202	rBV	4739704	6661583	52.42%	11.700%
9	17.324	2388	2395	2410	rBV	1702295	2475167	19.48%	4.347%
10	19.942	2834	2840	2860	rBV	10403622	12708197	100.00%	22.320%
11	21.495	3099	3104	3122	rBV	1637567	2393590	18.84%	4.204%
12	23.906	3508	3514	3529	rBV2	927038	2053748	16.16%	3.607%




Sum of corrected areas: 56935480

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034285.D
Acq On : 21 Mar 2022 10:47
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

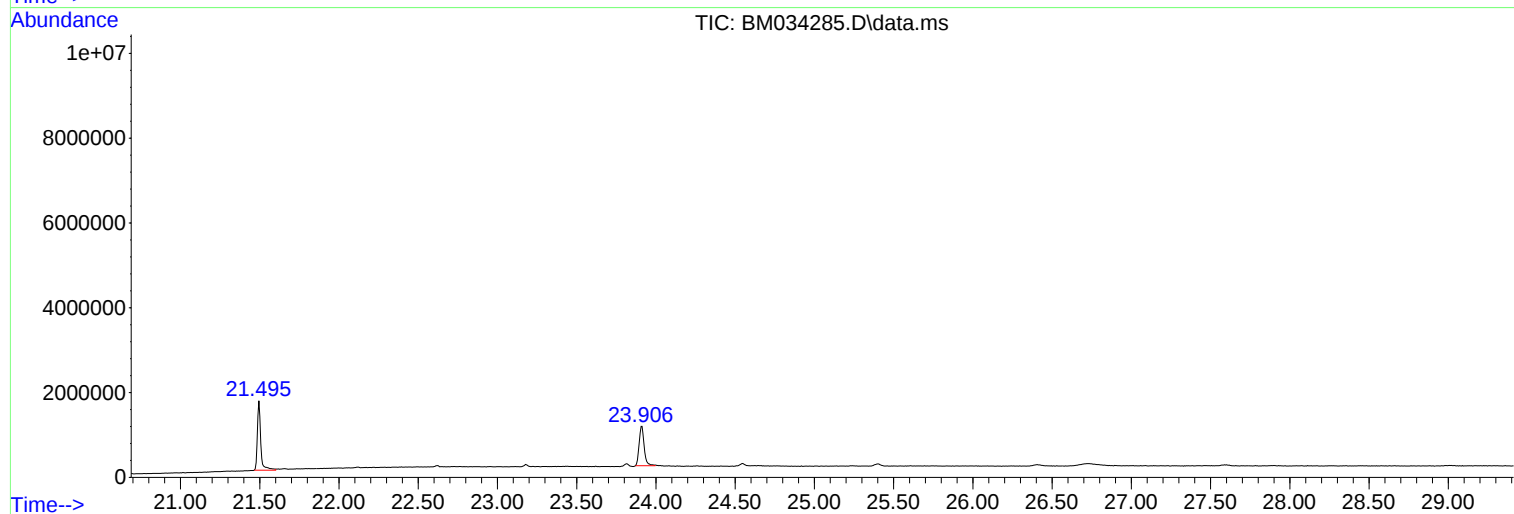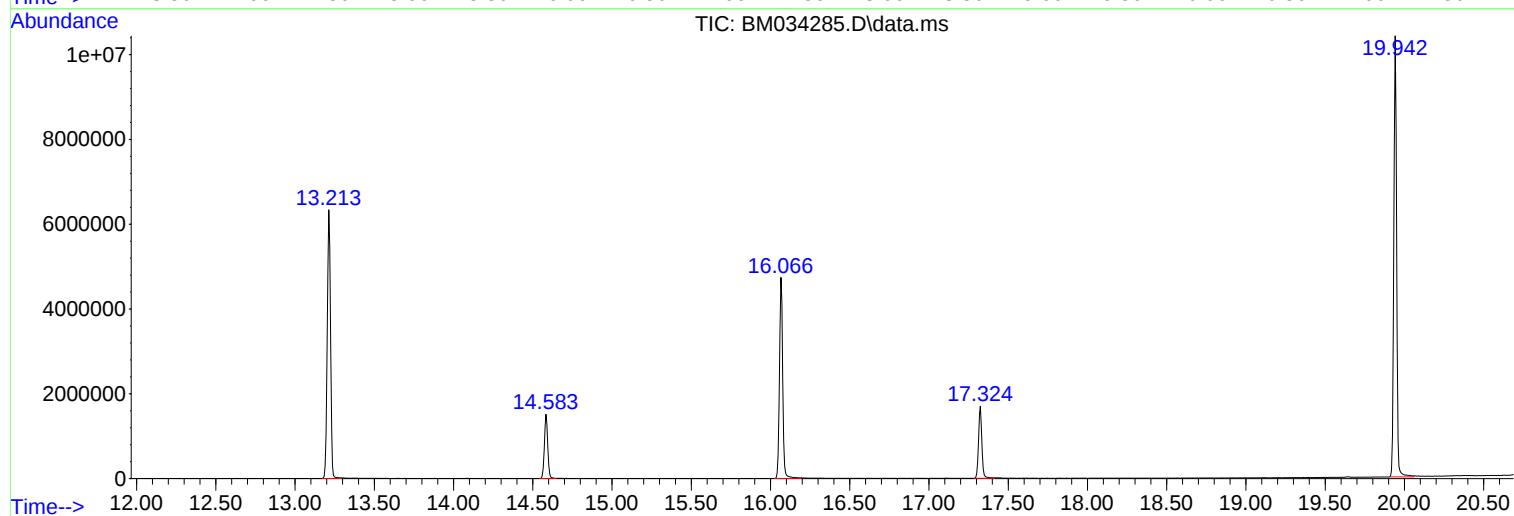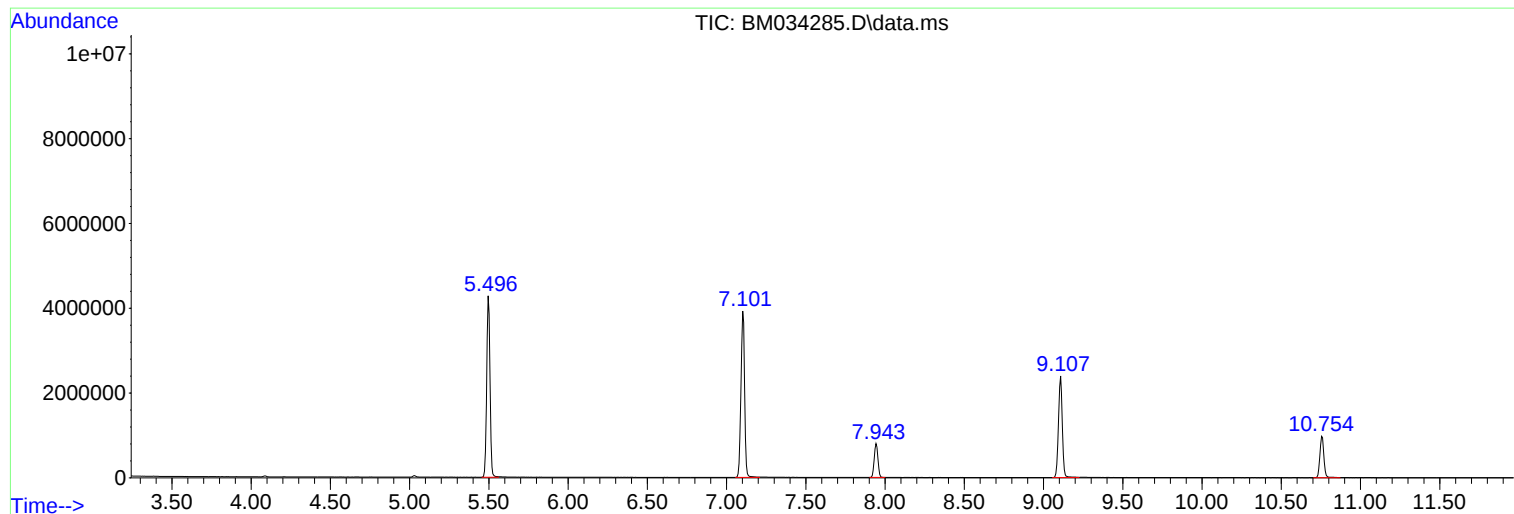

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034285.D
Acq On : 21 Mar 2022 10:47
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034285.D
Acq On : 21 Mar 2022 10:47
Operator : CG/JU
Sample : PB143392BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------