

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
 Data File : BM034291.D
 Acq On : 21 Mar 2022 17:03
 Operator : CG/JU
 Sample : PB143425BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143425BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.501	378	385	397	rBV	3909414	5820828	45.68%	10.415%
2	7.101	650	657	673	rBV	3664913	5990848	47.01%	10.719%
3	7.942	793	800	810	rBV	762481	1194880	9.38%	2.138%
4	9.107	990	998	1018	rBV	2289942	3857367	30.27%	6.902%
5	10.754	1271	1278	1288	rBV	918874	1609919	12.63%	2.880%
6	13.213	1689	1696	1707	rBV	6076362	8768297	68.80%	15.688%
7	14.583	1922	1929	1941	rBV	1490092	2170783	17.03%	3.884%
8	16.065	2174	2181	2198	rBV	4730881	6695203	52.54%	11.979%
9	17.324	2388	2395	2409	rBV	1611168	2484832	19.50%	4.446%
10	19.942	2834	2840	2860	rBV	10299405	12743909	100.00%	22.801%
11	21.495	3099	3104	3119	rBV	1630964	2395039	18.79%	4.285%
12	23.906	3507	3514	3532	rBV2	961450	2158946	16.94%	3.863%




Sum of corrected areas: 55890851

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034291.D
Acq On : 21 Mar 2022 17:03
Operator : CG/JU
Sample : PB143425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143425BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

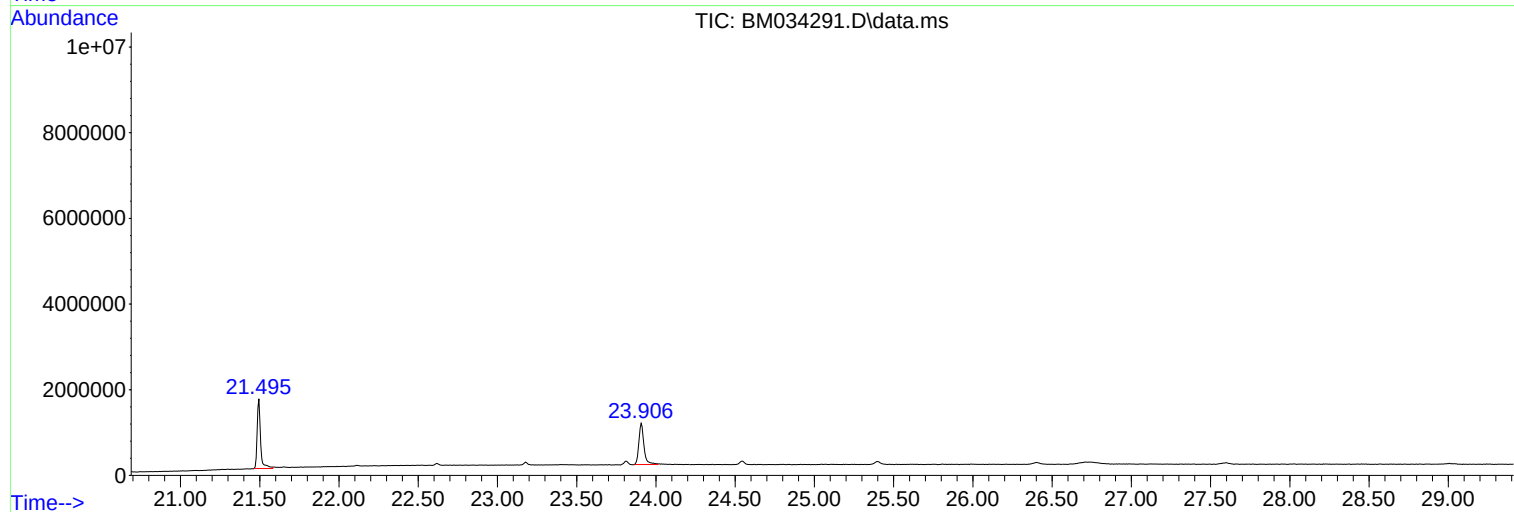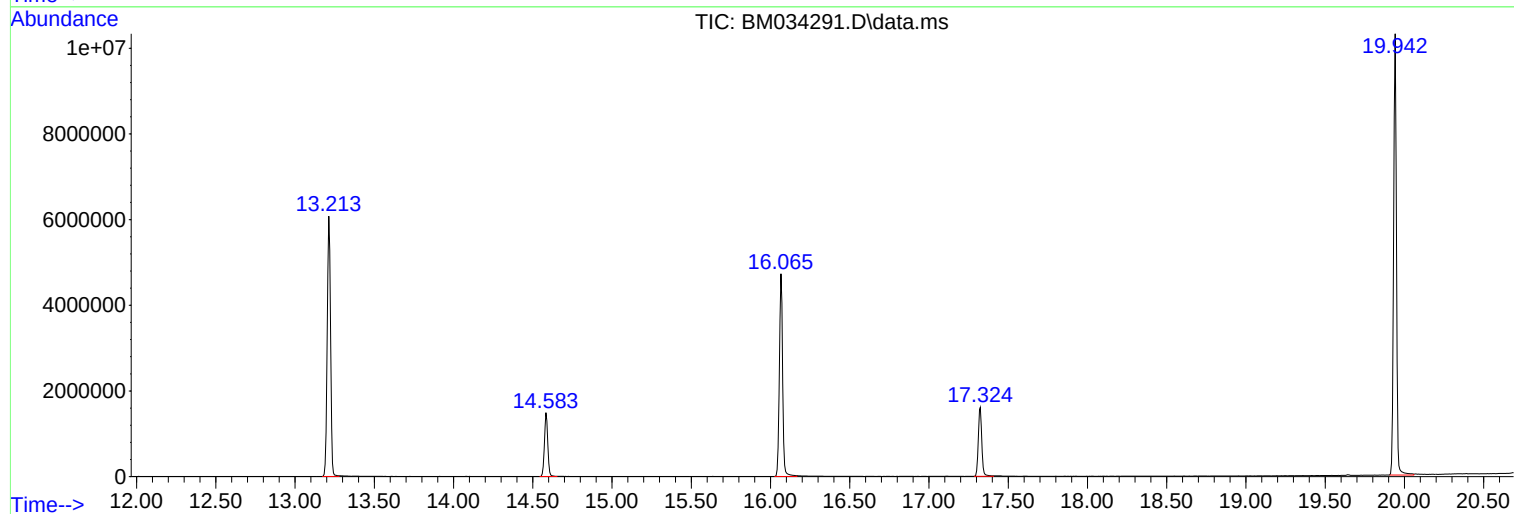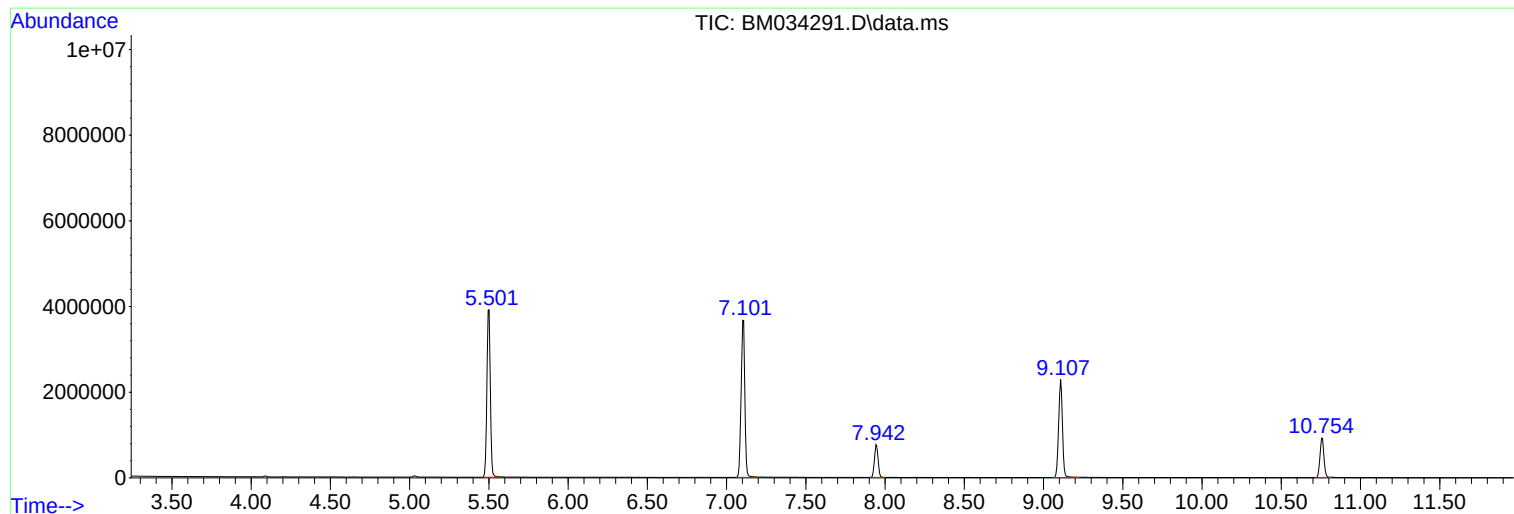

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034291.D
Acq On : 21 Mar 2022 17:03
Operator : CG/JU
Sample : PB143425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143425BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034291.D
Acq On : 21 Mar 2022 17:03
Operator : CG/JU
Sample : PB143425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143425BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------