
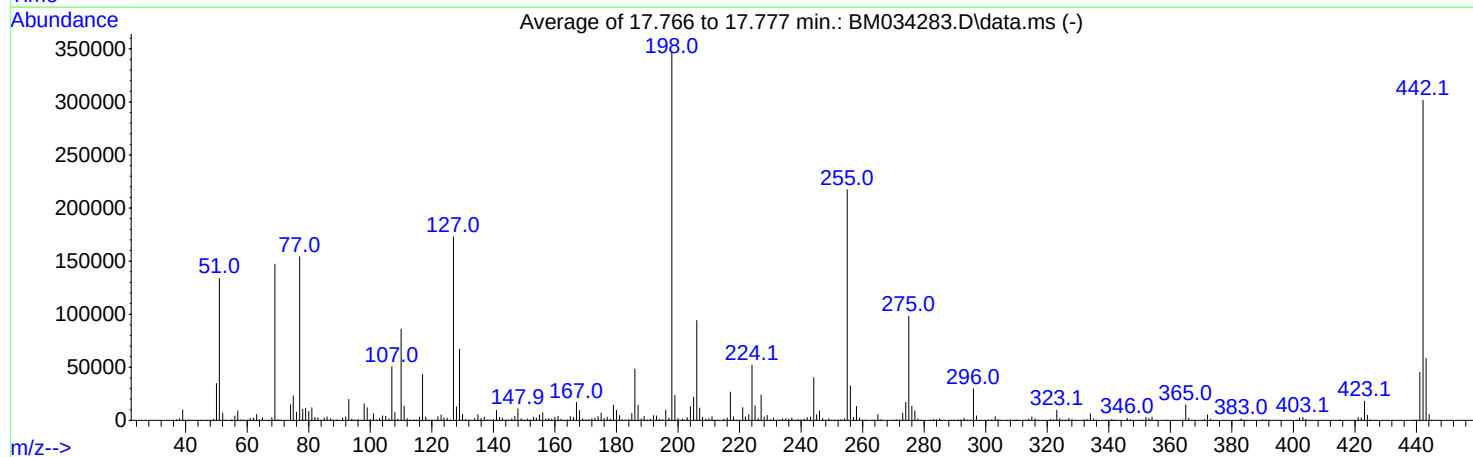


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
 Data File : BM034283.D
 Acq On : 21 Mar 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 16 02:38:26 2022

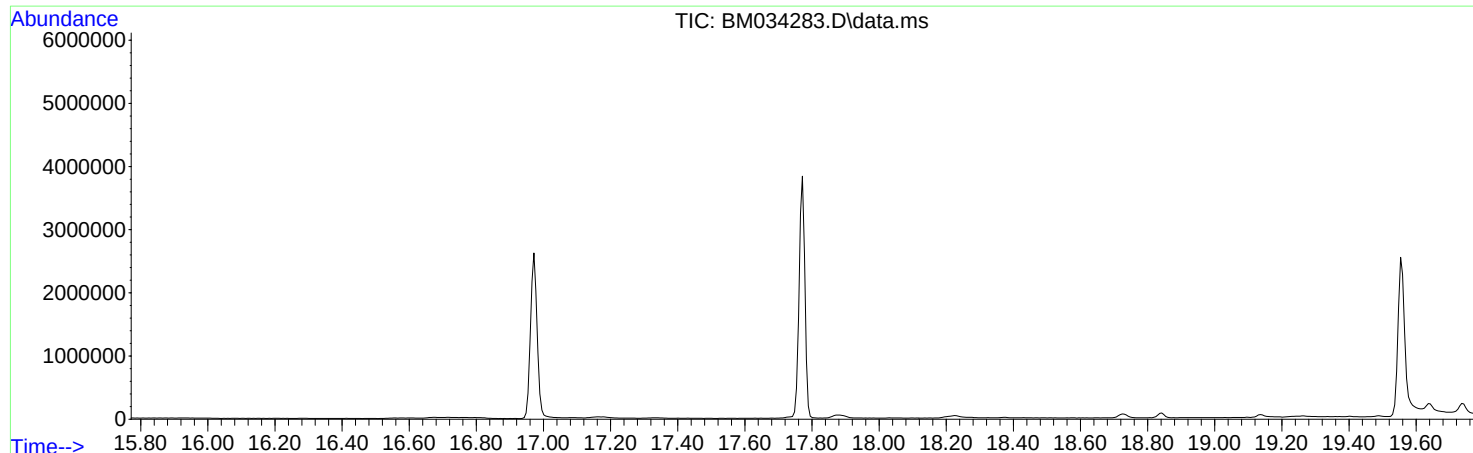




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	133722	PASS
68	69	0.00	2	1.8	2600	PASS
69	198	0.00	100	42.5	147141	PASS
70	69	0.00	2	0.6	844	PASS
127	198	10	80	49.9	172907	PASS
197	198	0.00	2	0.6	2075	PASS
198	198	100	100	100.0	346517	PASS
199	198	5	9	6.8	23597	PASS
275	198	10	60	28.3	98064	PASS
365	198	1	100	4.2	14570	PASS
441	198	0.01	100	13.1	45451	PASS
442	442	50	100	100.0	301525	PASS
443	442	15	24	19.4	58517	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034283.D
Acq On : 21 Mar 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 21 17:52:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

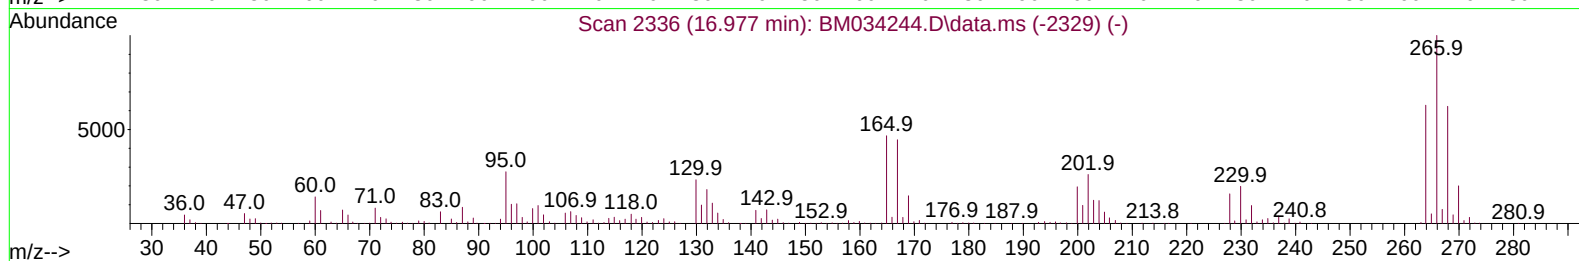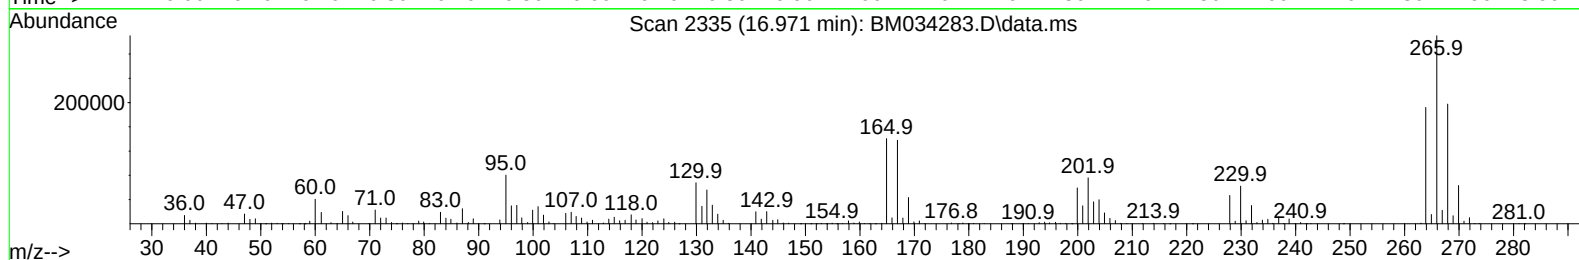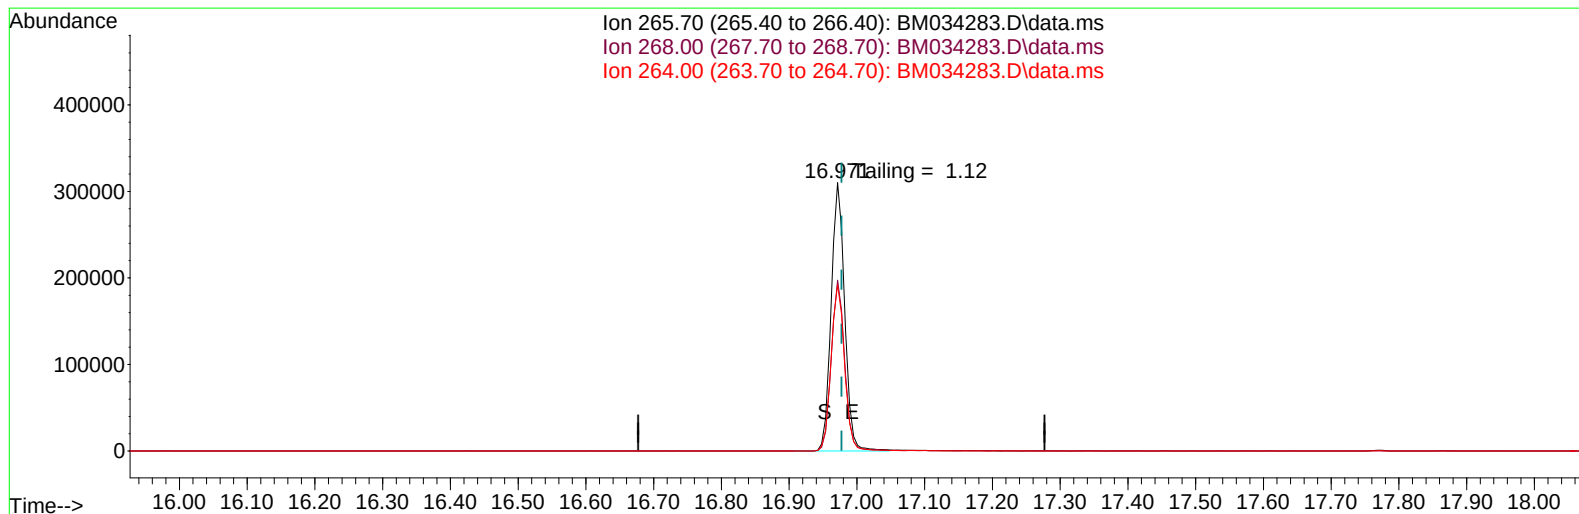

TIC: BM034283.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.006) 175994.66 ng




response 428598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.70
264.00	62.90	61.93
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\  
Data File : BM034283.D  
Acq On    : 21 Mar 2022  09:02  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 21 17:52:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

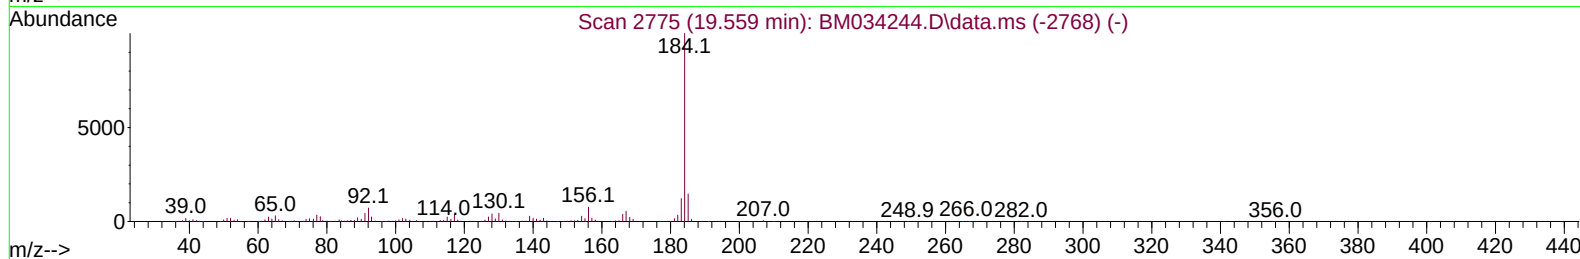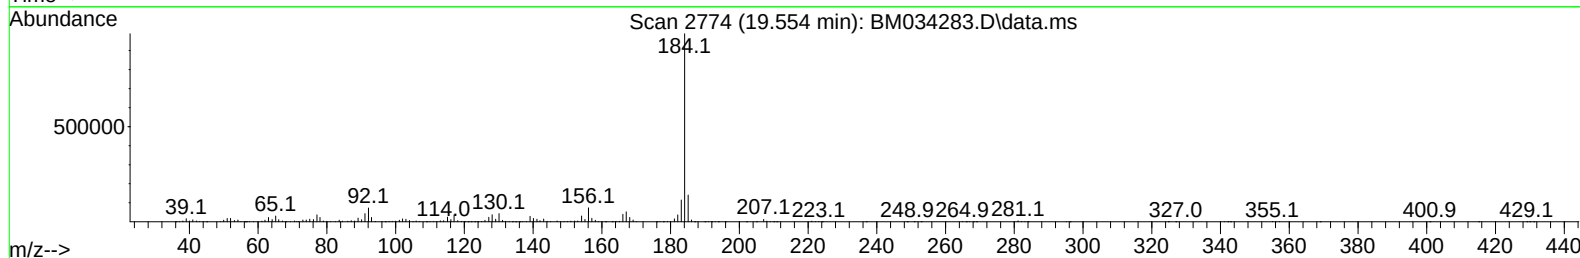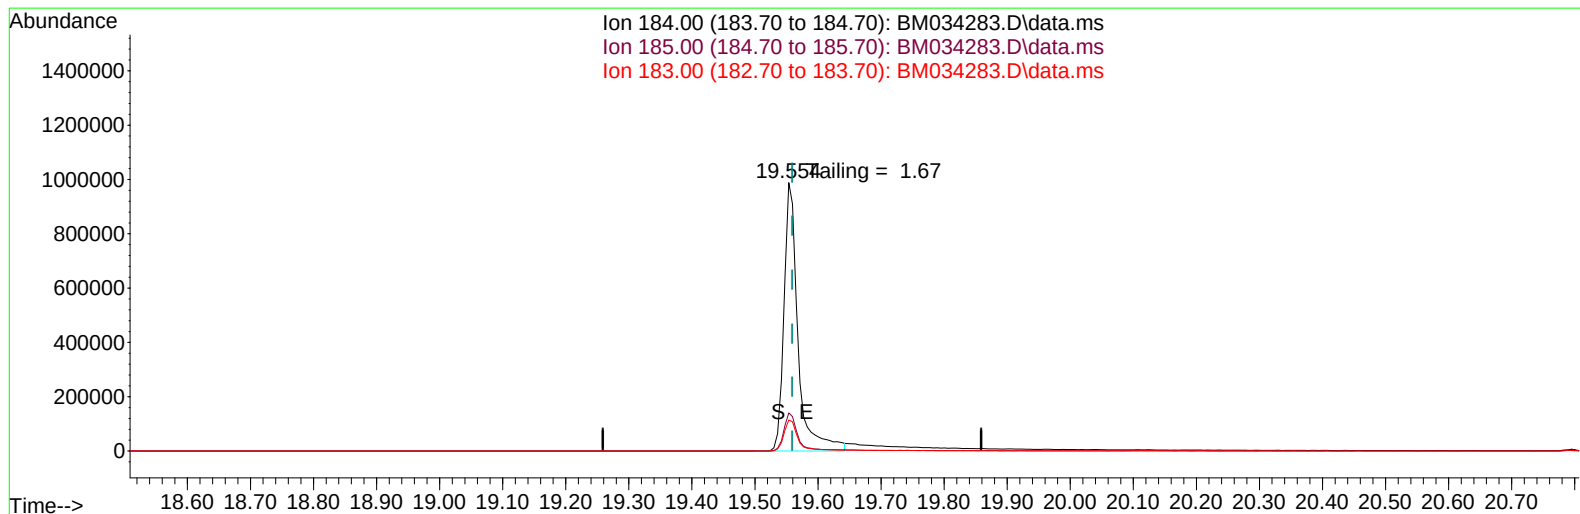

TIC: BM034283.D\data.ms

(77) Benzidine

19.554min (-0.005) 8062.90 ng

response **1694366**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.21
183.00	12.20	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/21/2022	BNA_M	<u>BM034283.D</u>
Compound Name	Response	Retention Time
DDT	1268242	20.79
DDD	5495	20.35
DDE	1740	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7235	1275477	0.57

Instrument :
BNA_M
ClientSampleId :
DFTPP