


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
 Data File : BM034289.D
 Acq On : 21 Mar 2022 15:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 16 02:38:26 2022

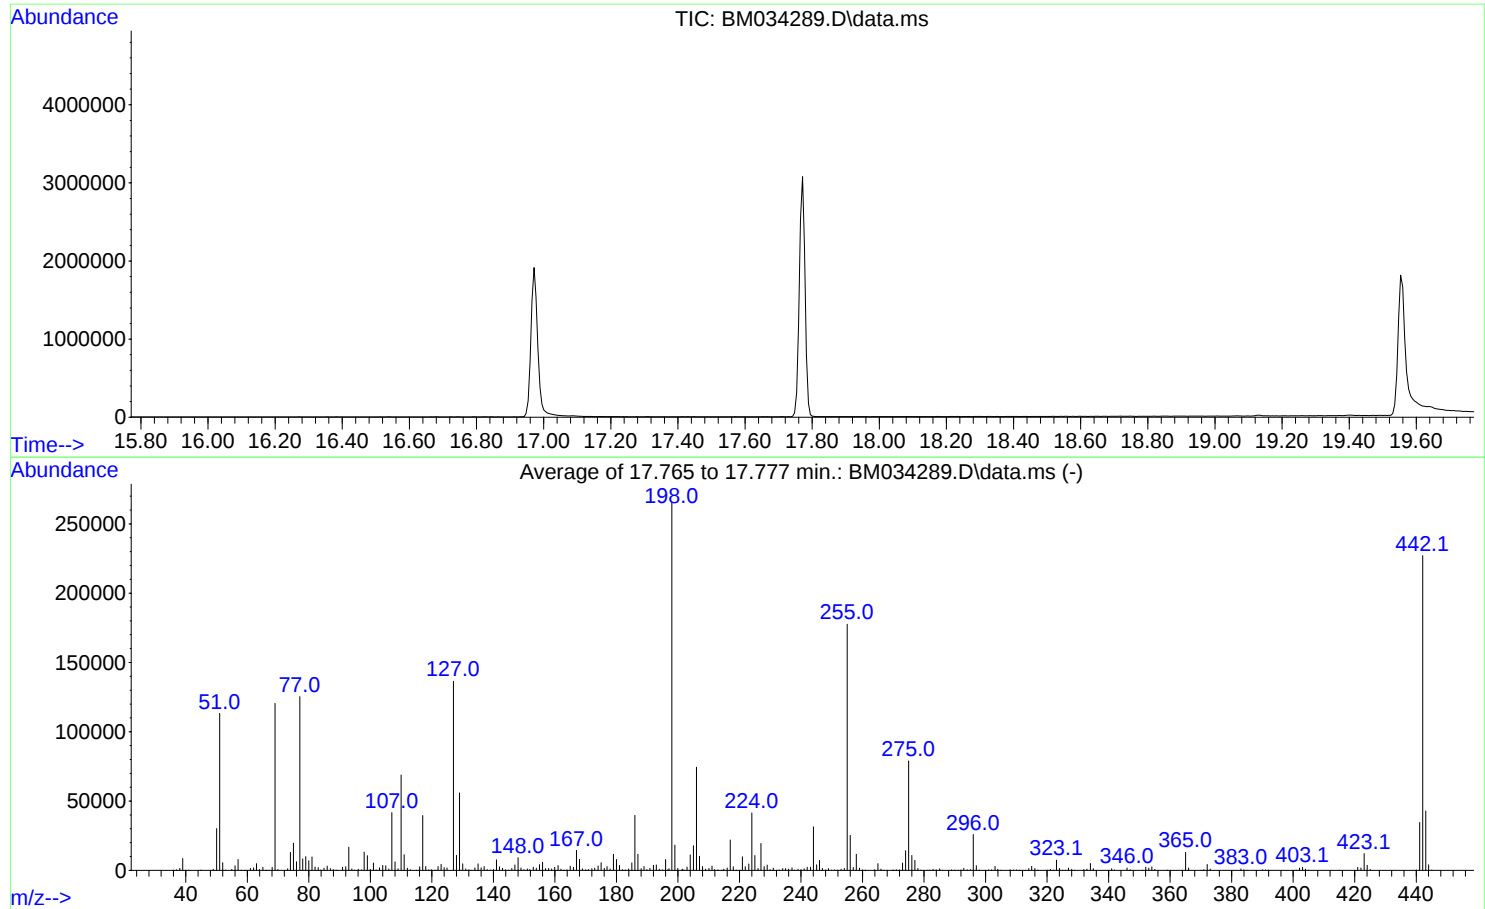




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	113259	PASS
68	69	0.00	2	1.8	2176	PASS
69	198	0.00	100	45.4	120565	PASS
70	69	0.00	2	0.5	555	PASS
127	198	10	80	51.4	136429	PASS
197	198	0.00	2	0.4	1108	PASS
198	198	100	100	100.0	265429	PASS
199	198	5	9	6.9	18279	PASS
275	198	10	60	29.7	78960	PASS
365	198	1	100	4.9	13049	PASS
441	198	0.01	100	13.0	34512	PASS
442	442	50	100	100.0	227115	PASS
443	442	15	24	18.9	42869	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
Data File : BM034289.D
Acq On : 21 Mar 2022 15:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 22 06:54:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

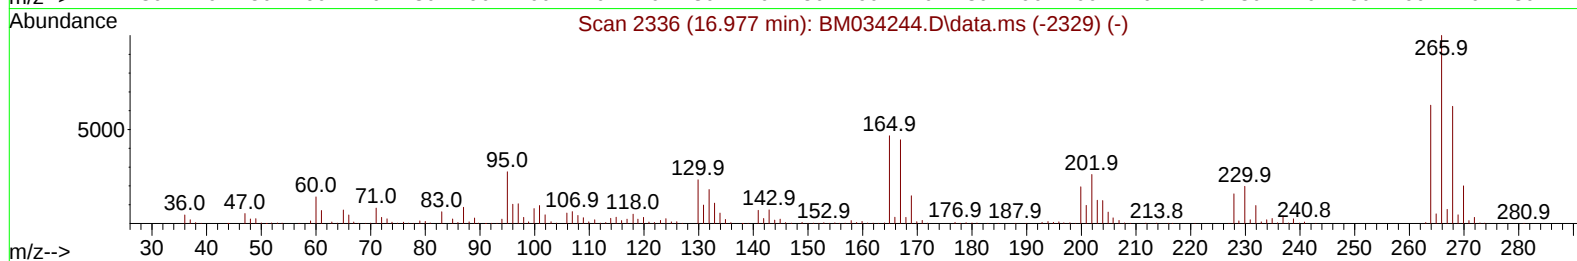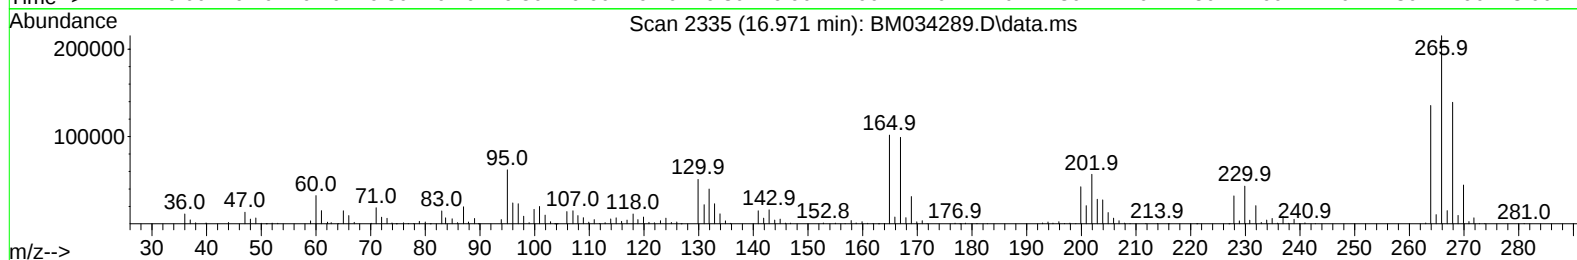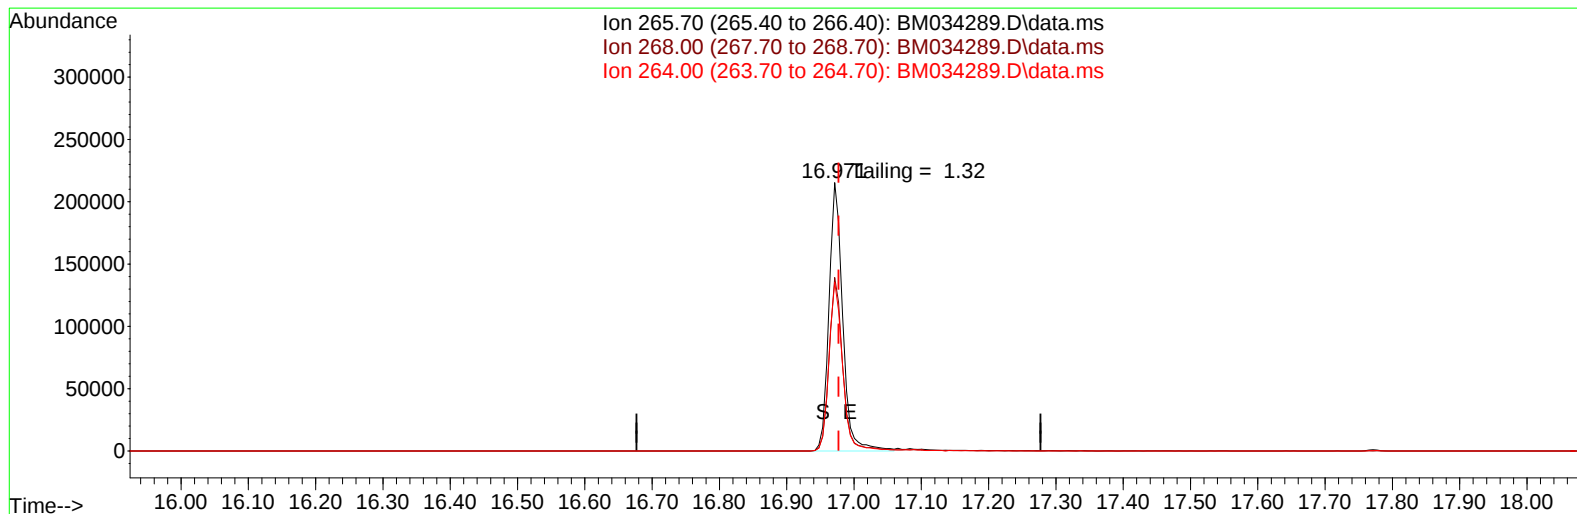

TIC: BM034289.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.006) 0.00 ng




response 308132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.61
264.00	62.90	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032122\
 Data File : BM034289.D
 Acq On : 21 Mar 2022 15:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 06:54:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 16 02:38:26 2022
 Response via : Initial Calibration

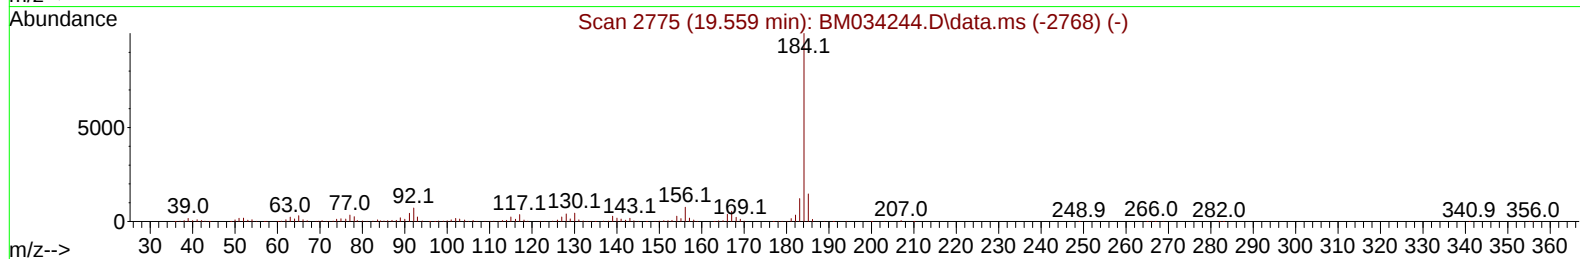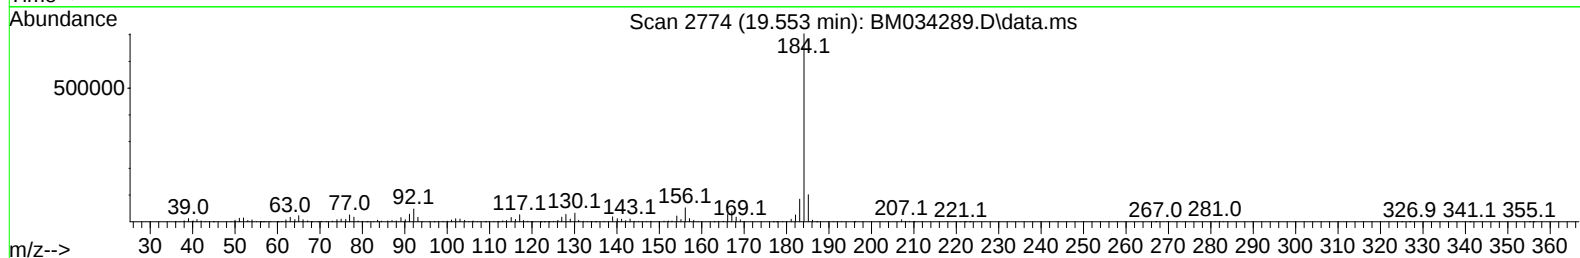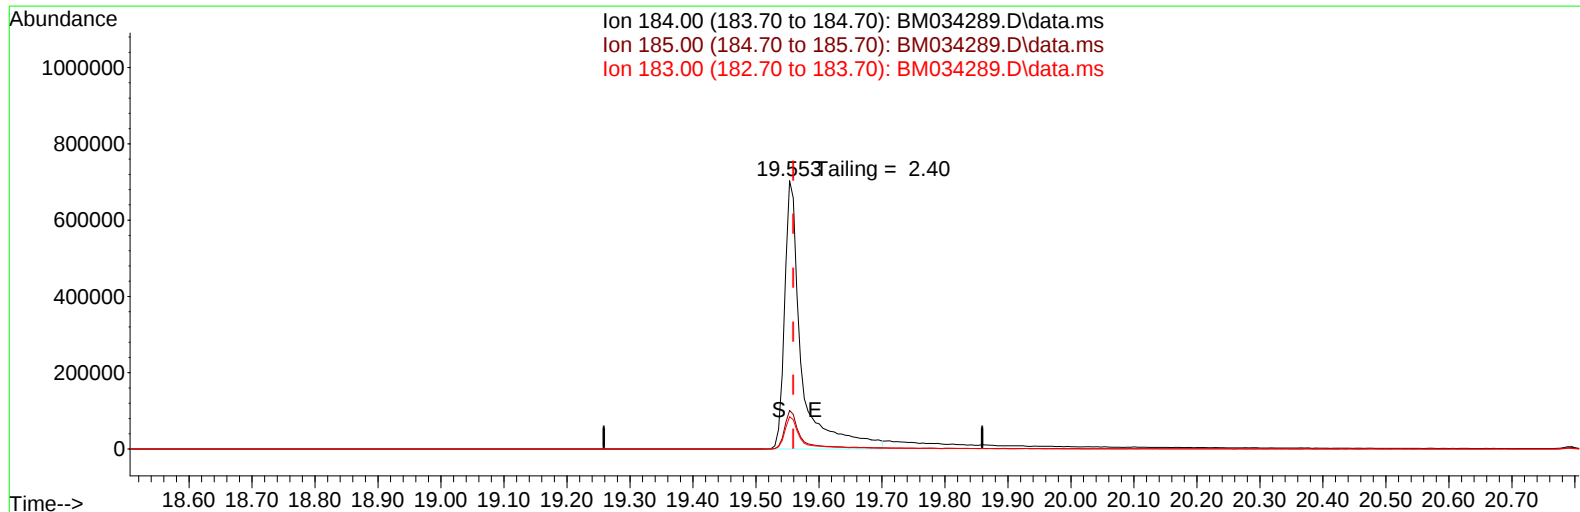

TIC: BM034289.D\data.ms

(77) Benzidine

19.553min (-0.006) 0.00 ng

response 1434553

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.37
183.00	12.20	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2022	BNA_M	<u>BM034289.D</u>
Compound Name	Response	Retention Time
DDT	1052861	20.794
DDD	9151	20.353
DDE	873	19.853
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10024	1062885	0.94

Instrument :
BNA_M
ClientSampleId :
DFTPP