
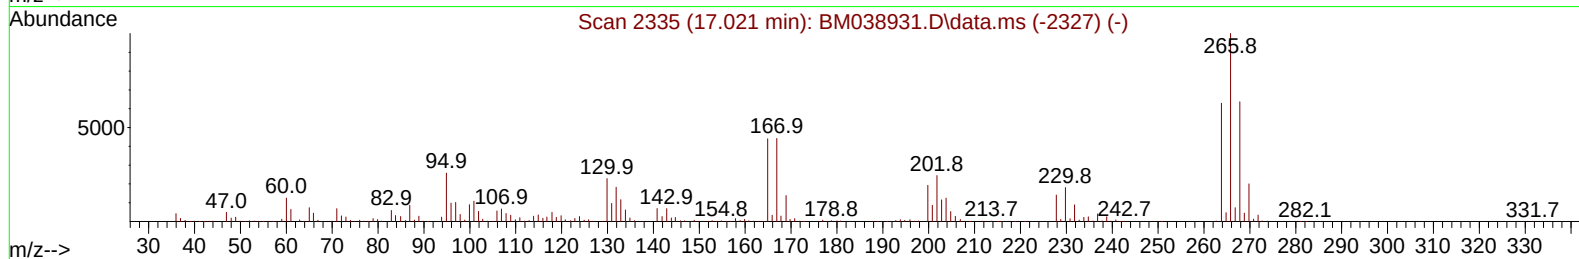
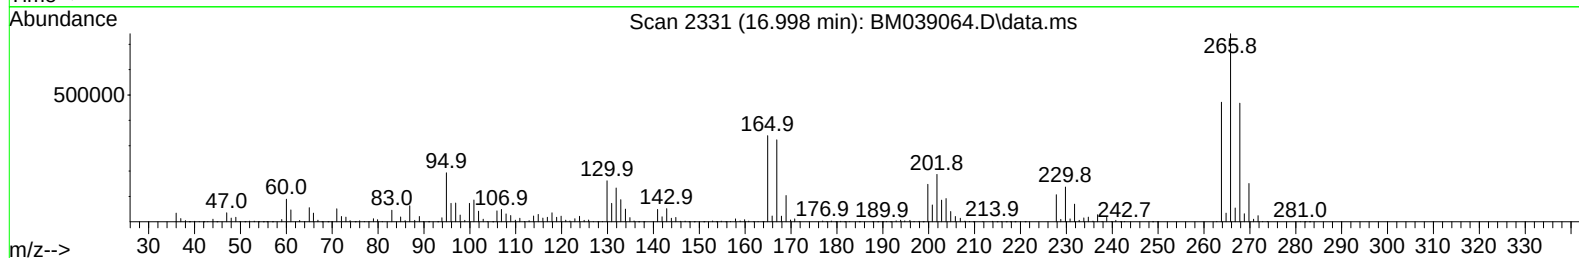


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032123\
Data File : BM039064.D
Acq On : 21 Mar 2023 11:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:59:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

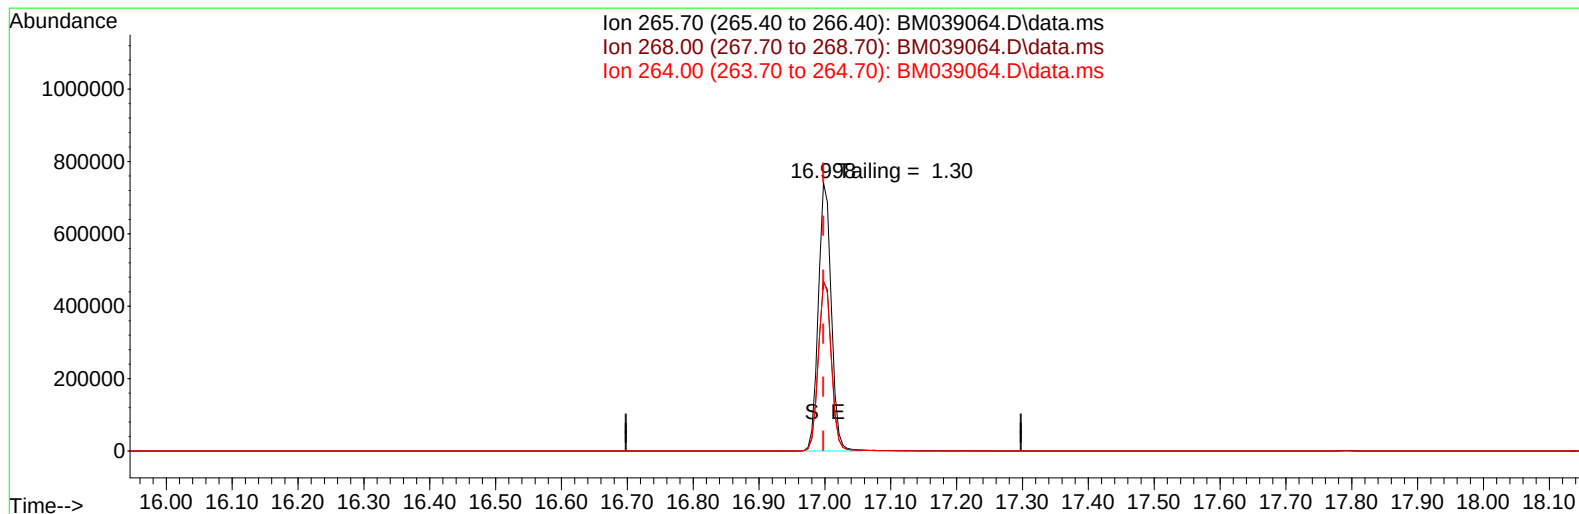

TIC: BM039064.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 232803.05 ng

response 1019270

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.04
264.00	62.90	63.56
0.00	0.00	0.00

