
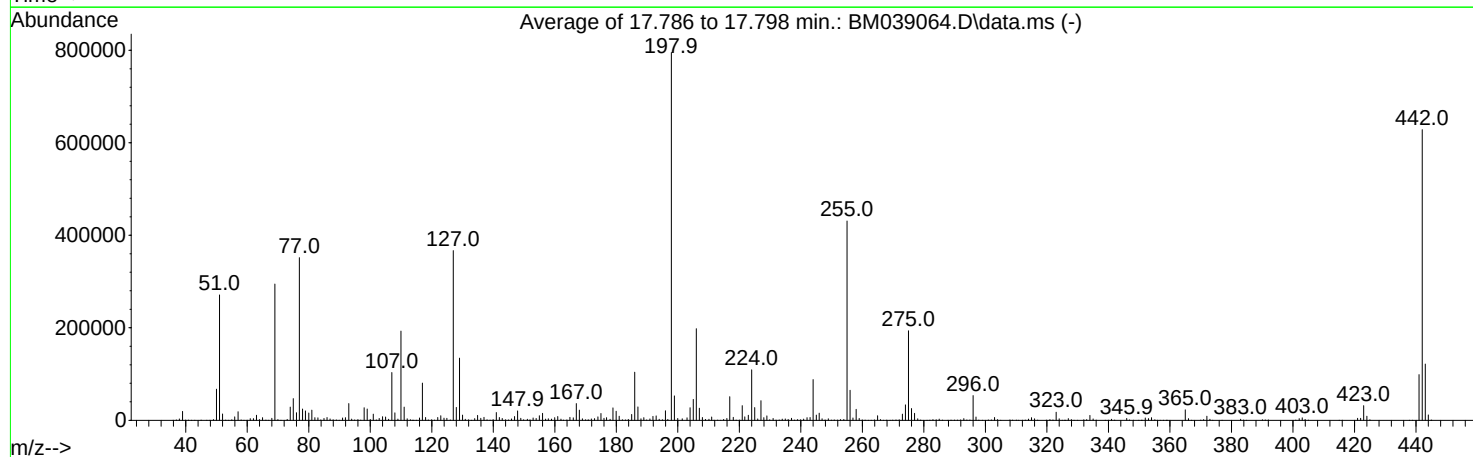


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032123\
 Data File : BM039064.D
 Acq On : 21 Mar 2023 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 22 03:36:20 2023

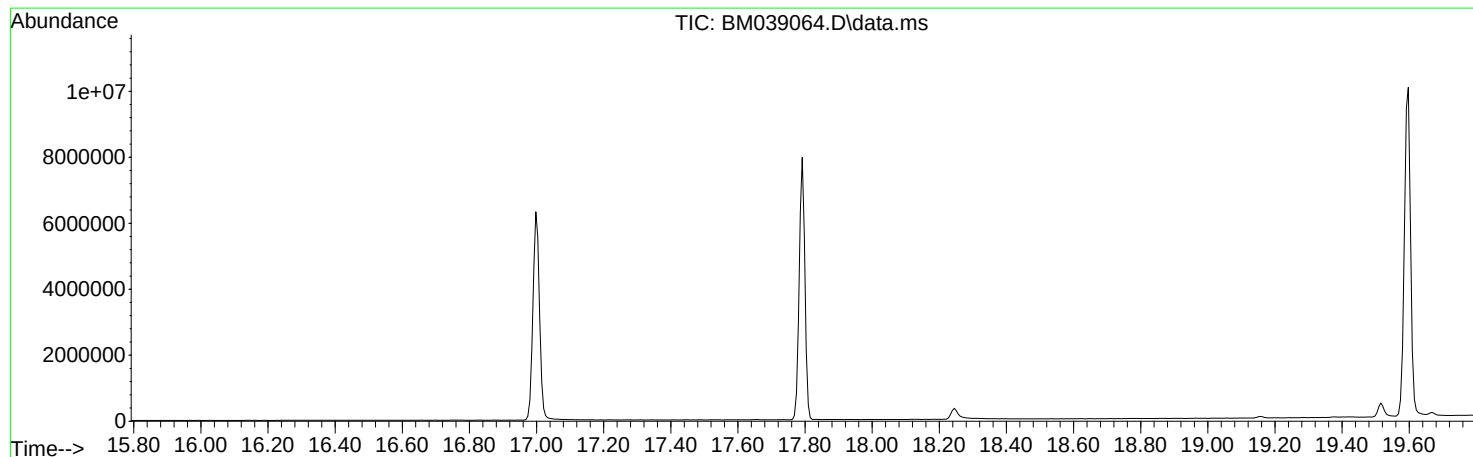




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	270967	PASS
68	69	0.00	2	1.5	4311	PASS
69	198	0.00	100	37.1	294677	PASS
70	69	0.00	2	0.6	1625	PASS
127	198	10	80	46.1	366827	PASS
197	198	0.00	2	0.2	1965	PASS
198	198	100	100	100.0	795307	PASS
199	198	5	9	6.7	52896	PASS
275	198	10	60	24.3	193557	PASS
365	198	1	100	2.9	22715	PASS
441	198	0.01	100	12.4	98693	PASS
442	442	50	100	100.0	628501	PASS
443	442	15	24	19.4	121773	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032123\
 Data File : BM039064.D
 Acq On : 21 Mar 2023 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 05:59:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 22 03:36:20 2023
 Response via : Initial Calibration

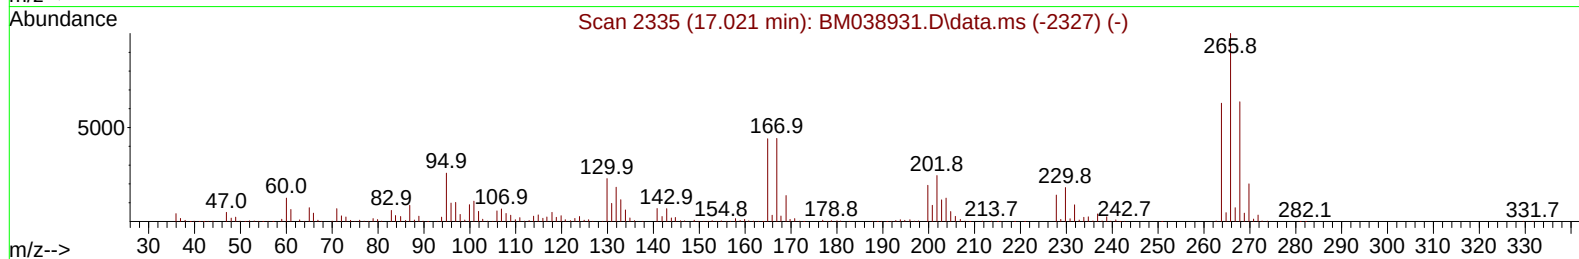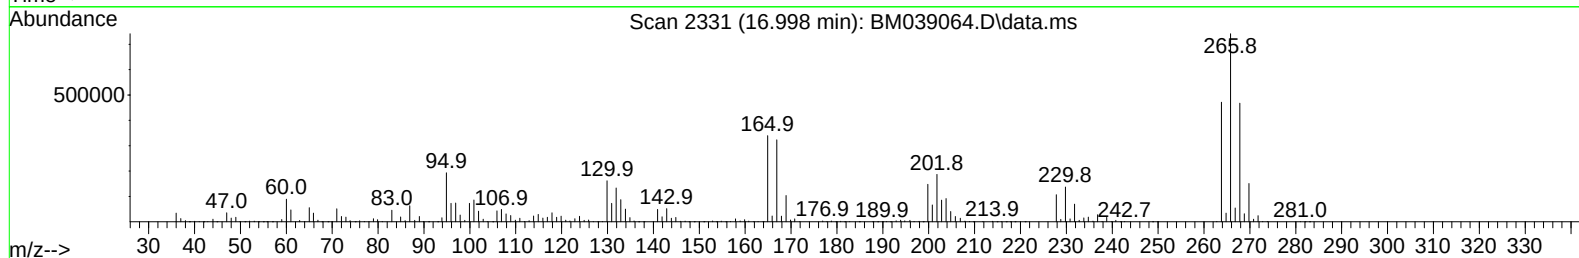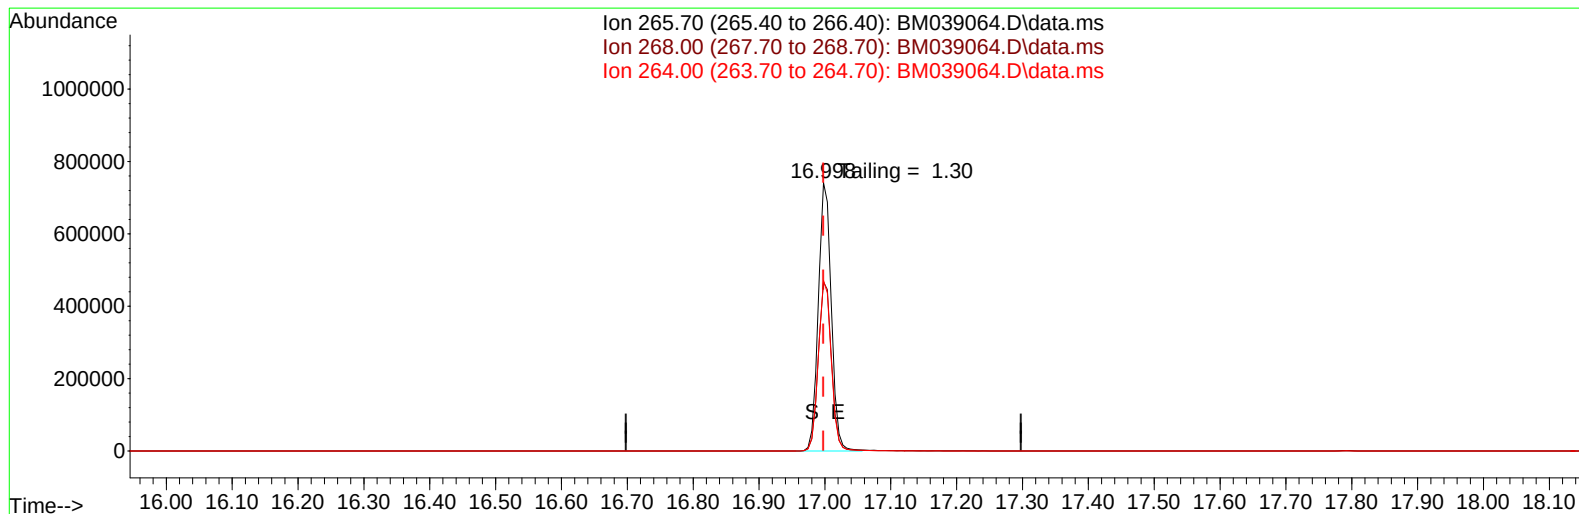

TIC: BM039064.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 232803.05 ng

response 1019270

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.04
264.00	62.90	63.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2023	BNA_M	<u>BM039064.D</u>
Compound Name	Response	Retention Time
DDT	2611621	20.827
DDD	31507	20.439
DDE	666	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32173	2643794	1.22

Instrument :
BNA_M
ClientSampleId :
DFTPP