
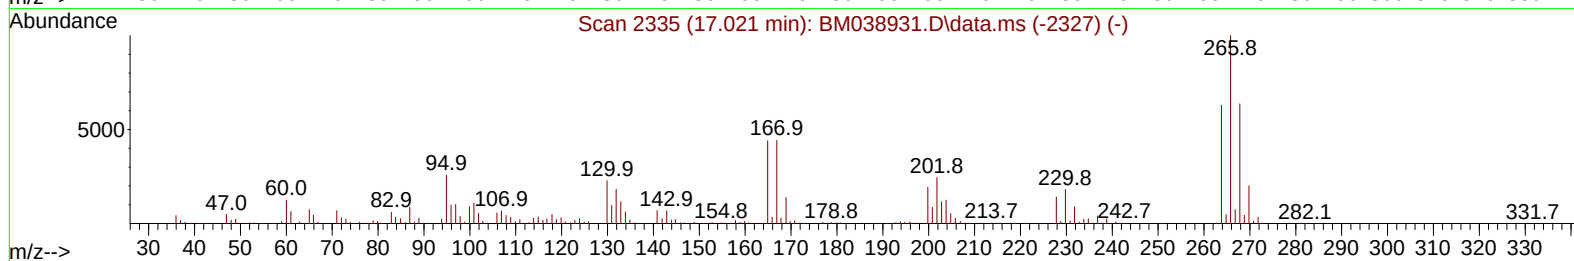
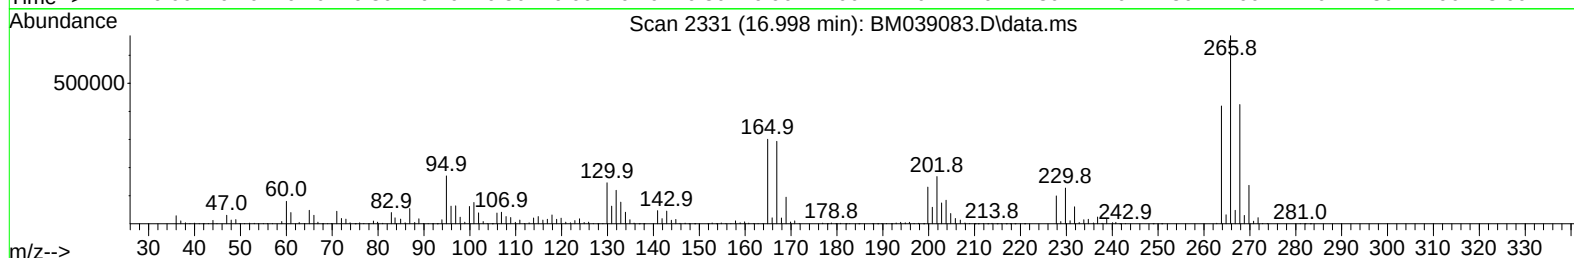


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039083.D
Acq On : 22 Mar 2023 09:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 06:52:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

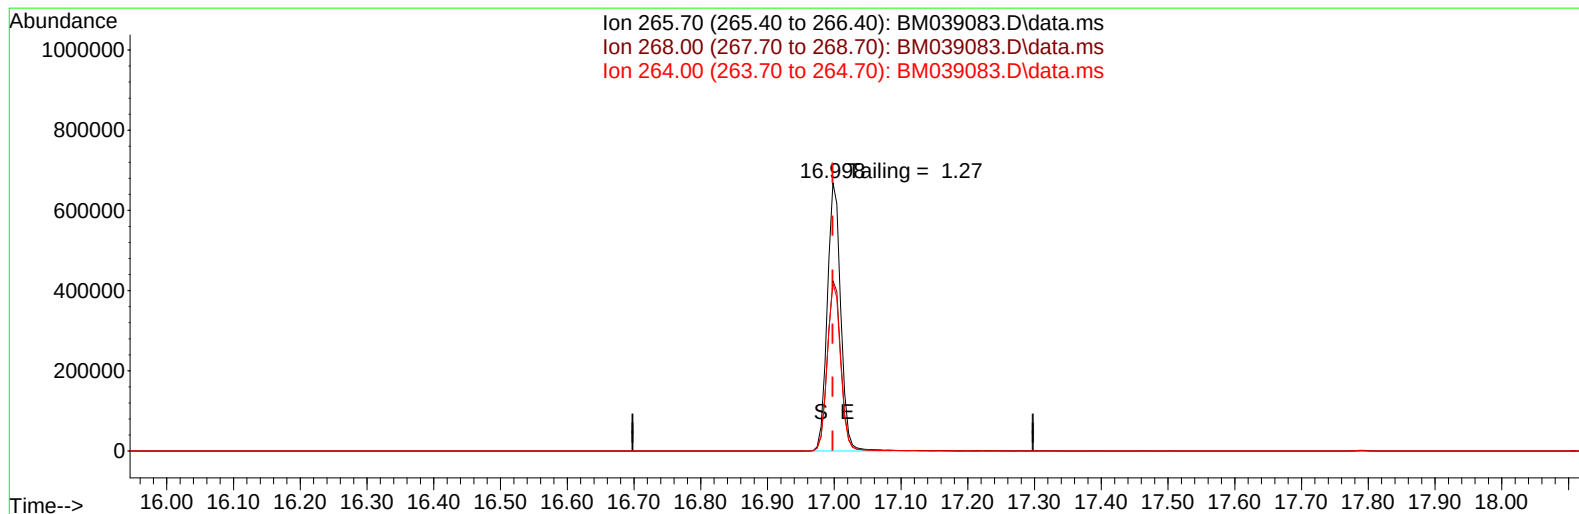

TIC: BM039083.D\data.ms

(70) Pentachlorophenol (C)




16.998min (+ 0.000) 740553.83 ng

response 940473

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.37
264.00	62.90	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039083.D
Acq On : 22 Mar 2023 09:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 06:52:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

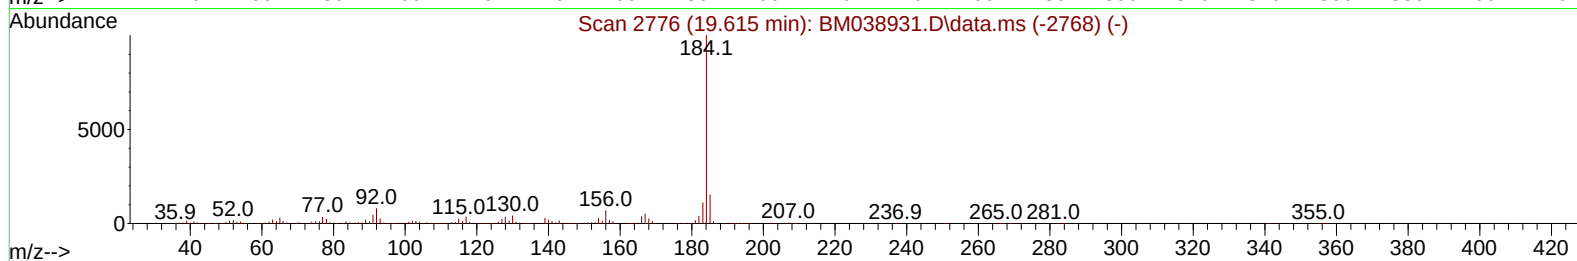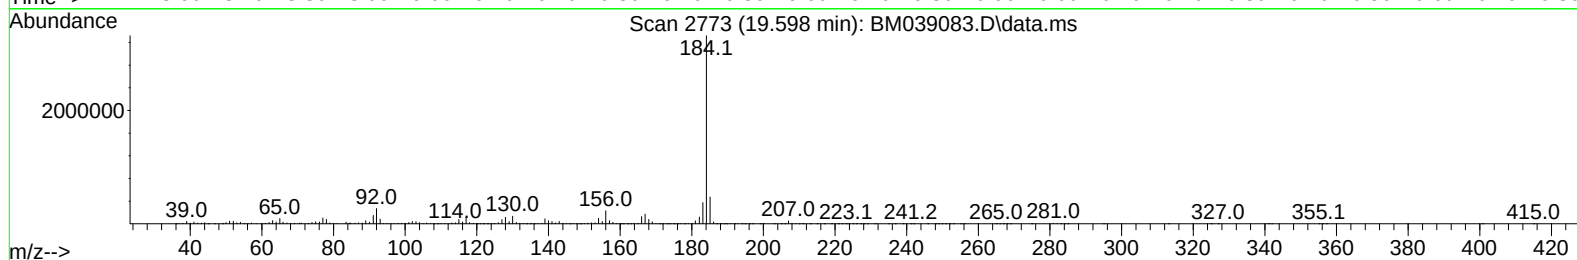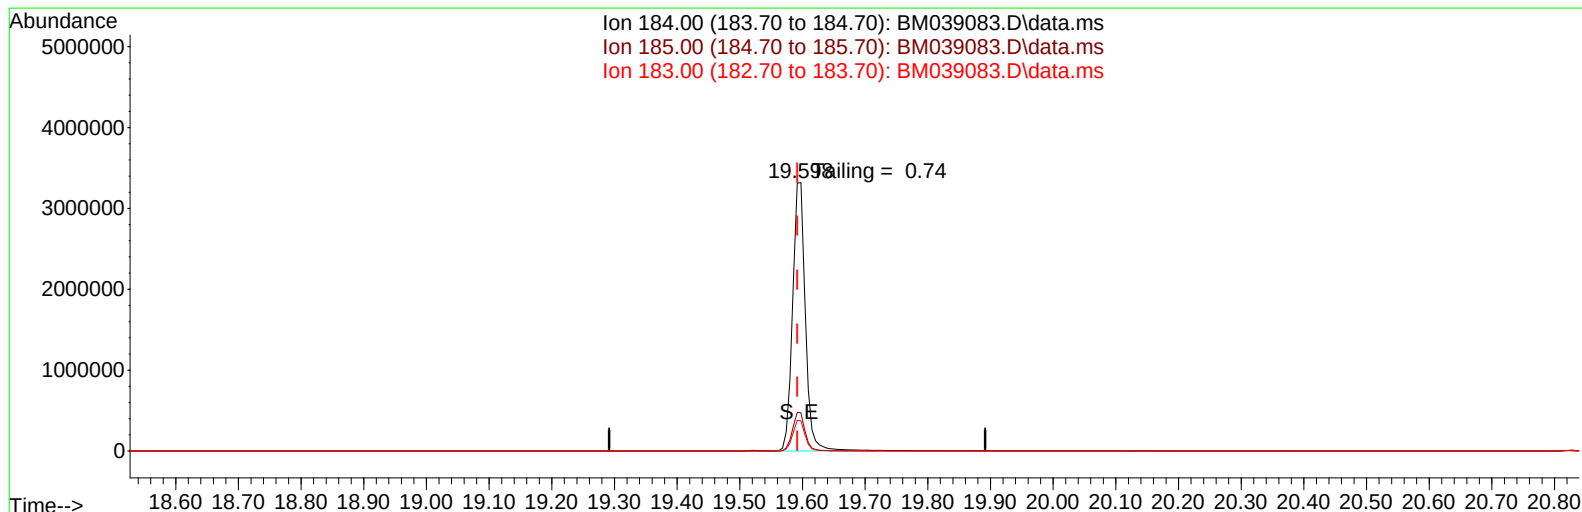

TIC: BM039083.D\data.ms

(77) Benzidine

19.598min (+ 0.006) 145058.19 ng

response 4773303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.23
183.00	11.00	11.26
0.00	0.00	0.00