

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
 Data File : BM039085.D
 Acq On : 22 Mar 2023 10:24
 Operator : CG/JU
 Sample : PB151573BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151573BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	294	301	310	rBV	3447420	4825300	20.88%	4.066%
2	5.522	373	380	392	rBV	8538592	12452202	53.88%	10.492%
3	7.134	645	654	674	rBV	8261822	13008936	56.29%	10.961%
4	7.963	788	795	806	rBV	1491430	2348794	10.16%	1.979%
5	9.134	985	994	1006	rBV	4807305	8096686	35.03%	6.822%
6	10.781	1266	1274	1284	rBV	1996956	3309706	14.32%	2.789%
7	13.233	1684	1691	1704	rBV	12193888	18469244	79.91%	15.561%
8	14.604	1917	1924	1935	rBV	3040358	4540519	19.65%	3.826%
9	16.092	2170	2177	2199	rBV	9028155	13665789	59.13%	11.514%
10	17.351	2384	2391	2403	rBV	3740491	5293958	22.91%	4.460%
11	18.245	2538	2543	2564	rBV2	217700	507653	2.20%	0.428%
12	19.515	2756	2759	2769	rBV3	133746	259326	1.12%	0.218%
13	19.974	2831	2837	2842	rBV	18323327	23111978	100.00%	19.473%
14	21.527	3097	3101	3110	rBV	3565139	4626595	20.02%	3.898%
15	23.962	3509	3515	3528	rVB2	2097165	4169364	18.04%	3.513%




Sum of corrected areas: 118686050

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039085.D
Acq On : 22 Mar 2023 10:24
Operator : CG/JU
Sample : PB151573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151573BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

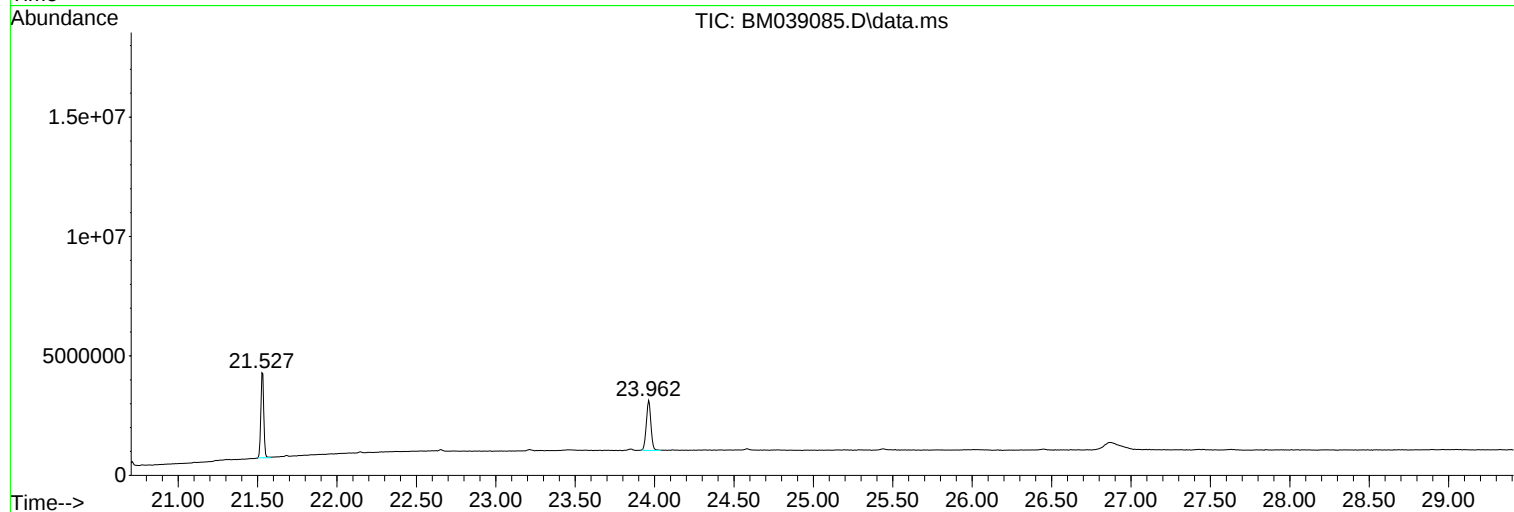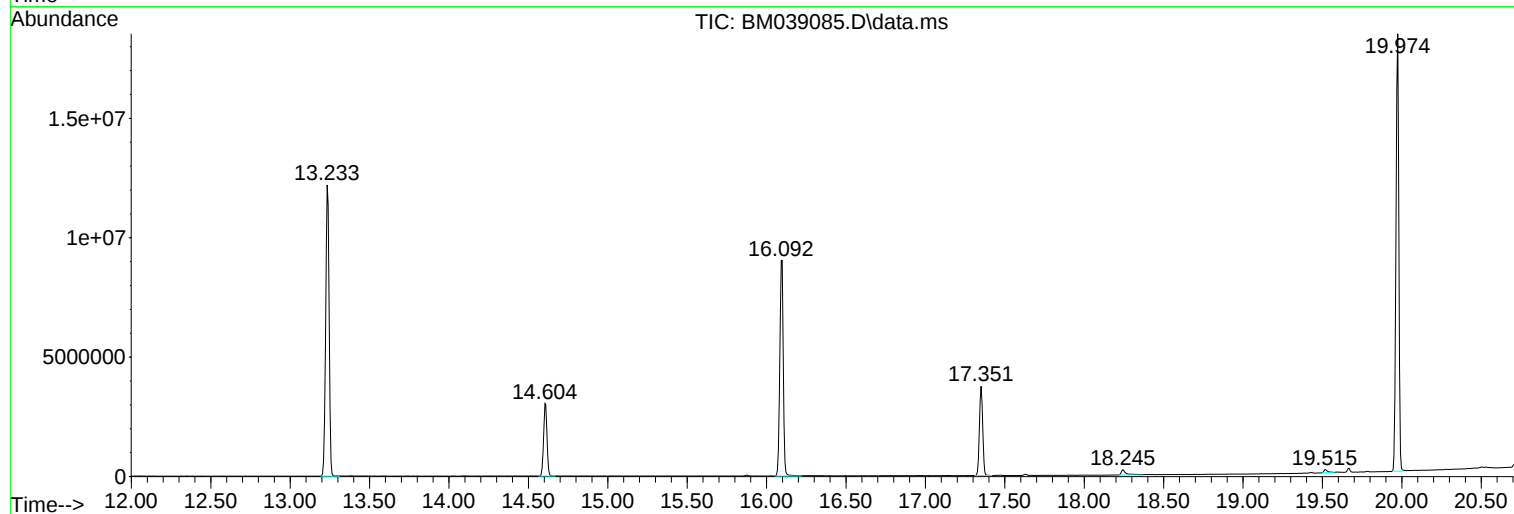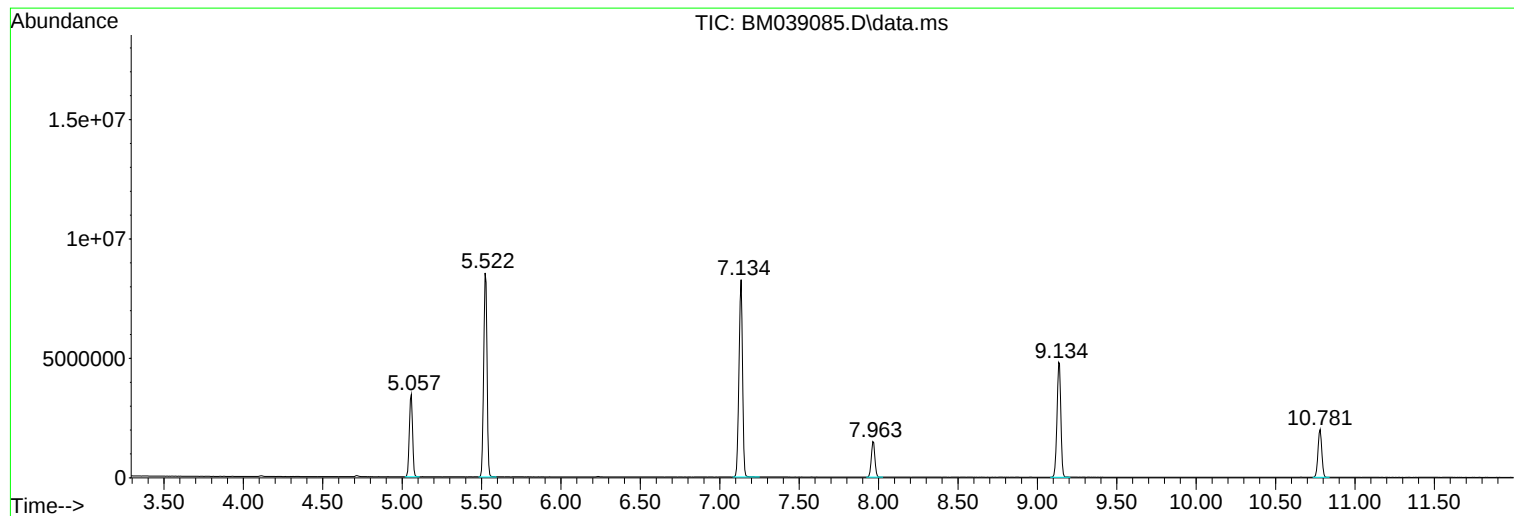

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039085.D
Acq On : 22 Mar 2023 10:24
Operator : CG/JU
Sample : PB151573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151573BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.057	41.09 ng	4825300	1,4-Dichlorobenzene-d4	7.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

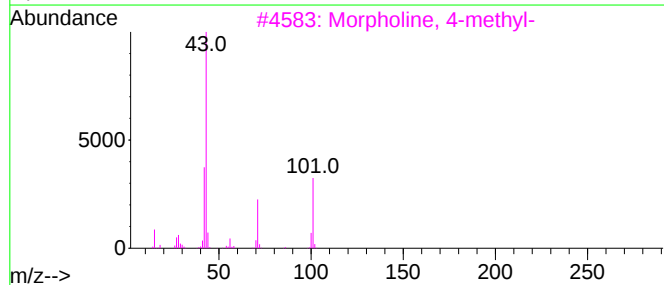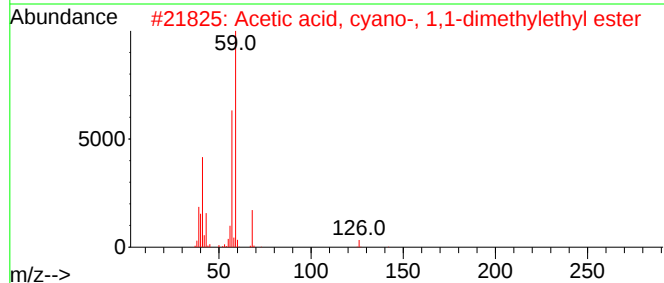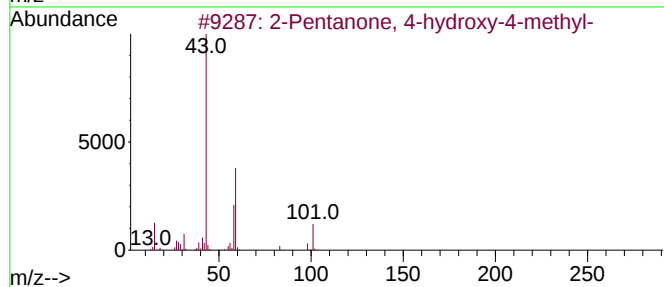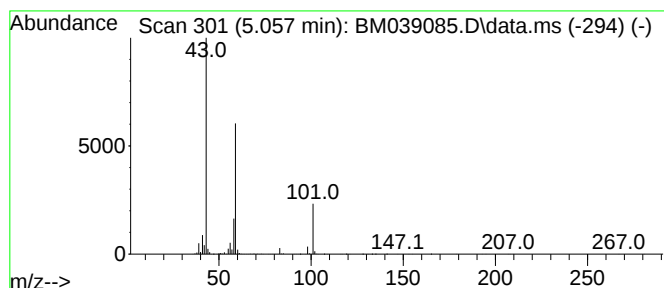

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039085.D
Acq On : 22 Mar 2023 10:24
Operator : CG/JU
Sample : PB151573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151573BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.057	41.1	ng	4825300	1	7.963	2348790	20.0