
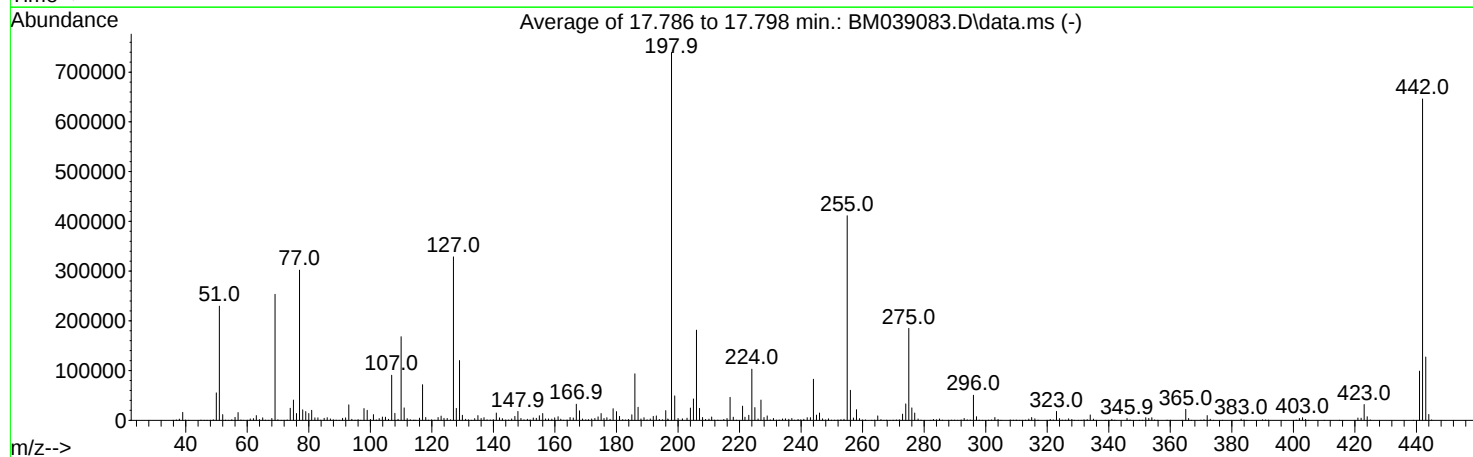


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
 Data File : BM039083.D
 Acq On : 22 Mar 2023 09:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 22 03:36:20 2023

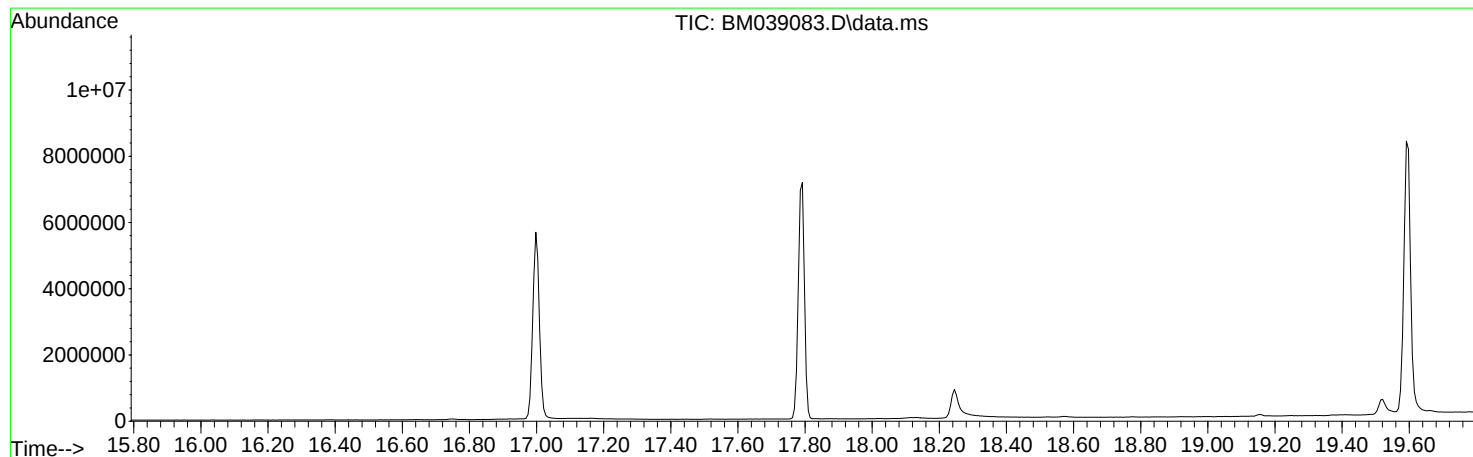




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	229588	PASS
68	69	0.00	2	1.4	3665	PASS
69	198	0.00	100	34.2	253277	PASS
70	69	0.00	2	0.5	1191	PASS
127	198	10	80	44.5	328768	PASS
197	198	0.00	2	0.4	2617	PASS
198	198	100	100	100.0	739627	PASS
199	198	5	9	6.6	49029	PASS
275	198	10	60	25.0	184683	PASS
365	198	1	100	3.0	22088	PASS
441	198	0.01	100	13.4	99027	PASS
442	442	50	100	100.0	646272	PASS
443	442	15	24	19.7	127125	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\  
Data File : BM039083.D  
Acq On    : 22 Mar 2023  09:09  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 23 06:52:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

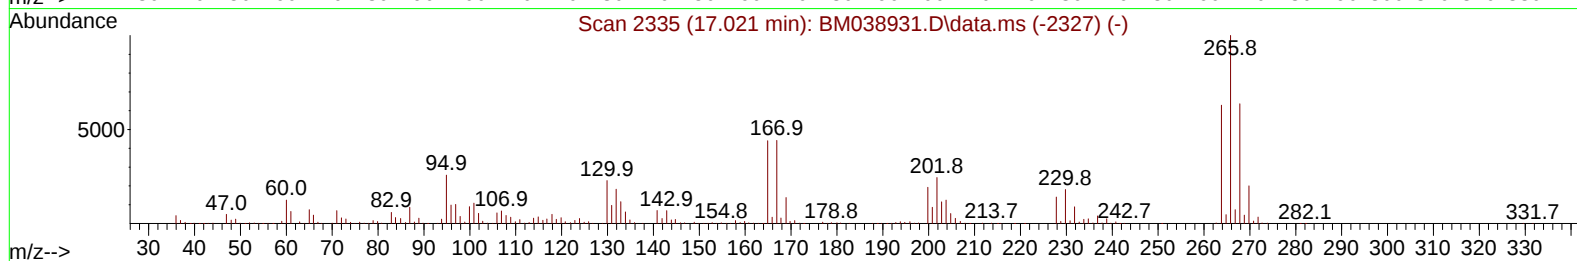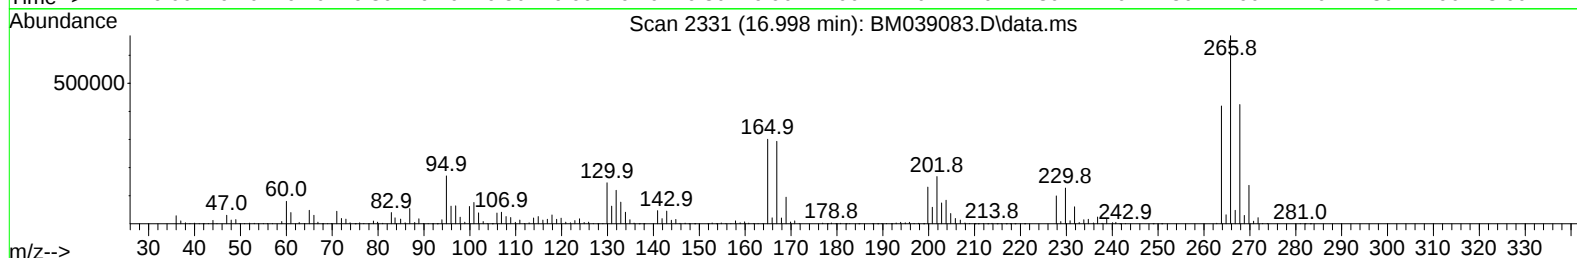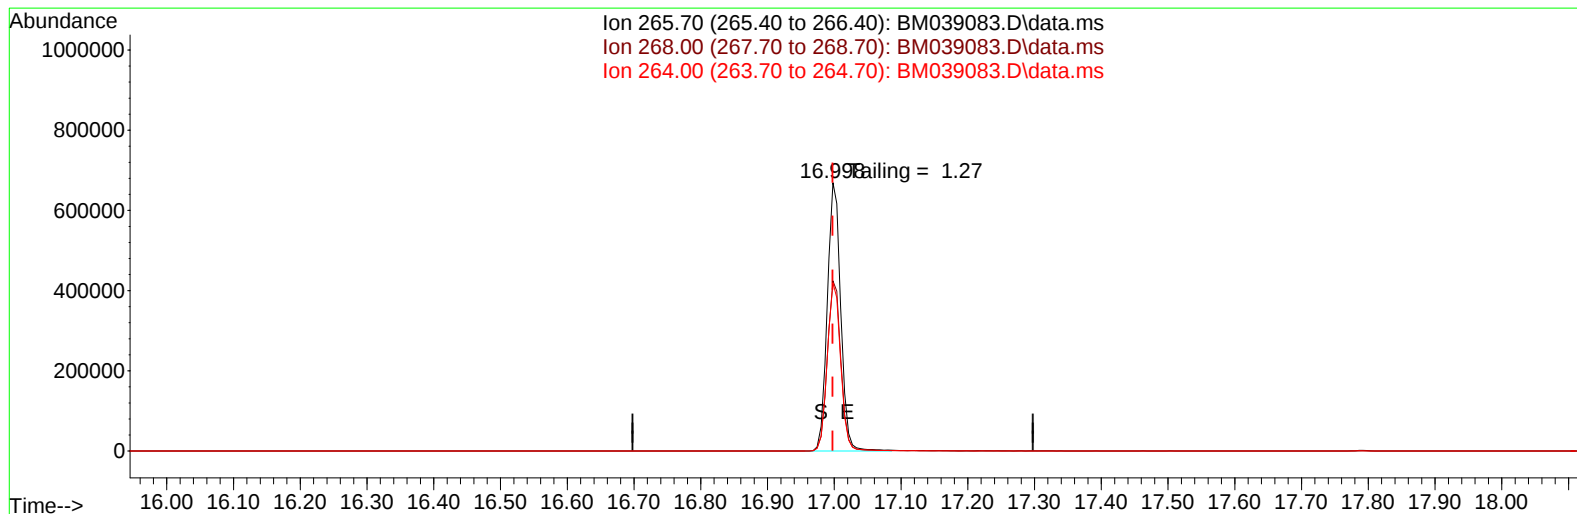

TIC: BM039083.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 740553.83 ng




response **940473**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.37
264.00	62.90	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
 Data File : BM039083.D
 Acq On : 22 Mar 2023 09:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 06:52:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 22 03:36:20 2023
 Response via : Initial Calibration

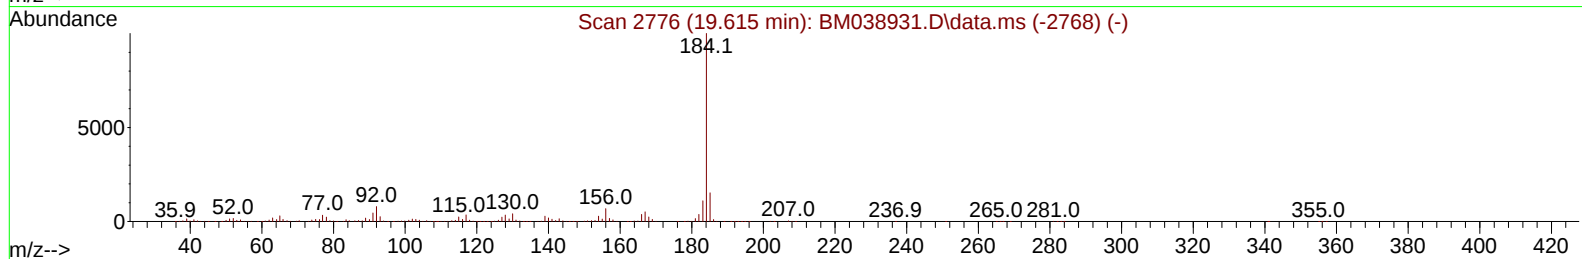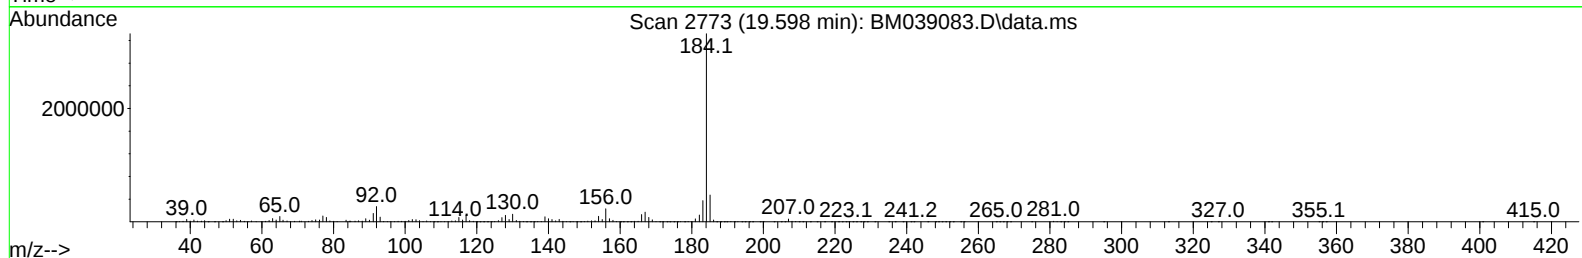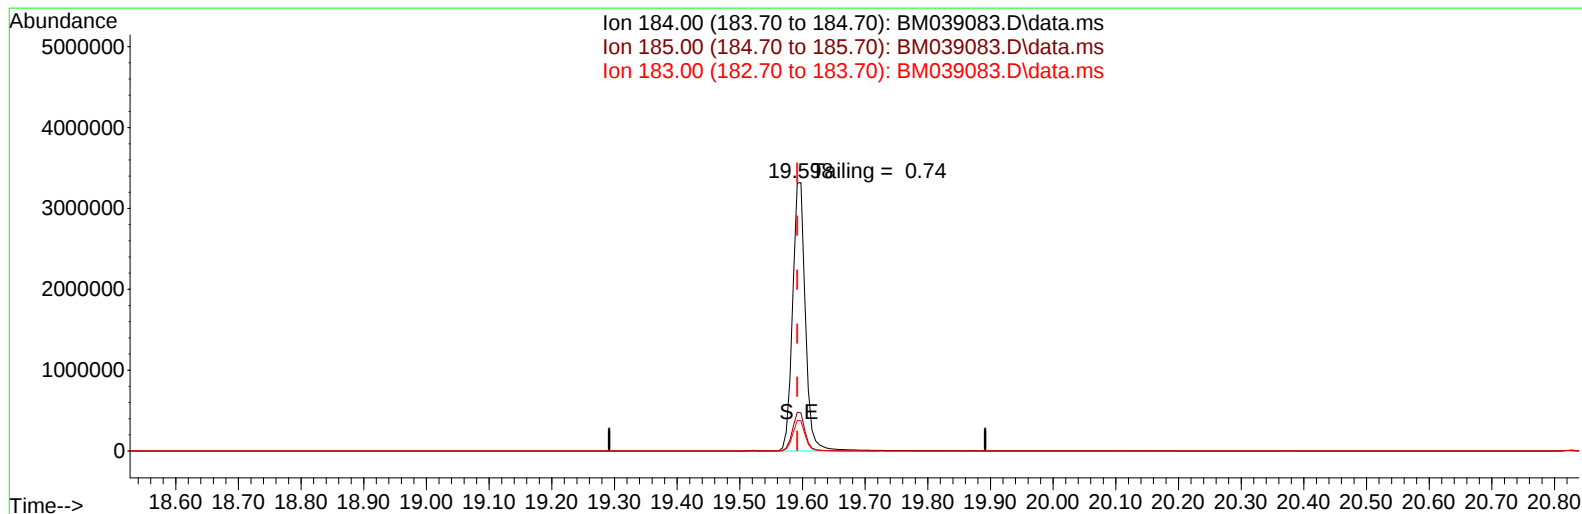

TIC: BM039083.D\data.ms

(77) Benzidine**19.598min (+ 0.006) 145058.19 ng****response 4773303**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.23
183.00	11.00	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2023	BNA_M	<u>BM039083.D</u>
Compound Name	Response	Retention Time
DDT	2623096	20.827
DDD	46507	20.439
DDE	2507	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49014	2672110	1.83

Instrument :
BNA_M
ClientSampleId :
DFTPP