


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039092.D
Acq On : 22 Mar 2023 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 22 03:36:20 2023

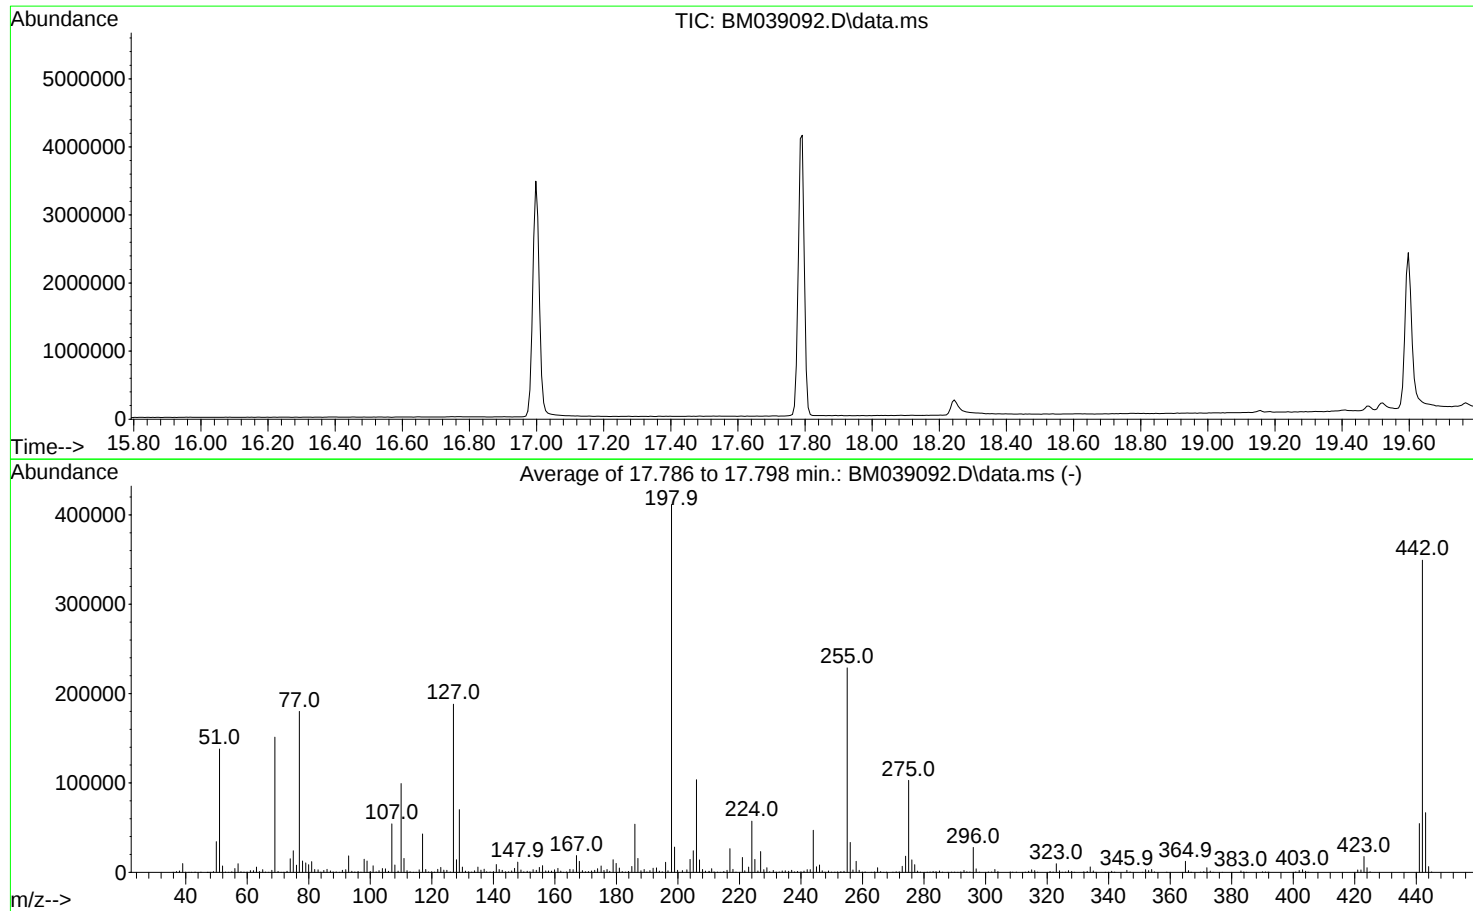




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	138084	PASS
68	69	0.00	2	1.5	2311	PASS
69	198	0.00	100	36.7	151194	PASS
70	69	0.00	2	0.6	934	PASS
127	198	10	80	45.7	188216	PASS
197	198	0.00	2	0.4	1640	PASS
198	198	100	100	100.0	411733	PASS
199	198	5	9	6.9	28269	PASS
275	198	10	60	25.0	102909	PASS
365	198	1	100	3.0	12336	PASS
441	198	0.01	100	13.3	54616	PASS
442	442	50	100	100.0	349397	PASS
443	442	15	24	19.1	66747	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039092.D
Acq On : 22 Mar 2023 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 23 06:53:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

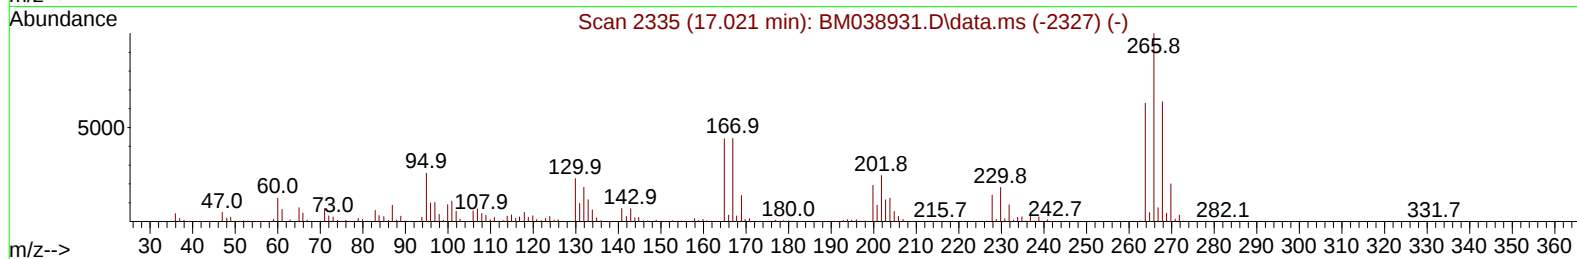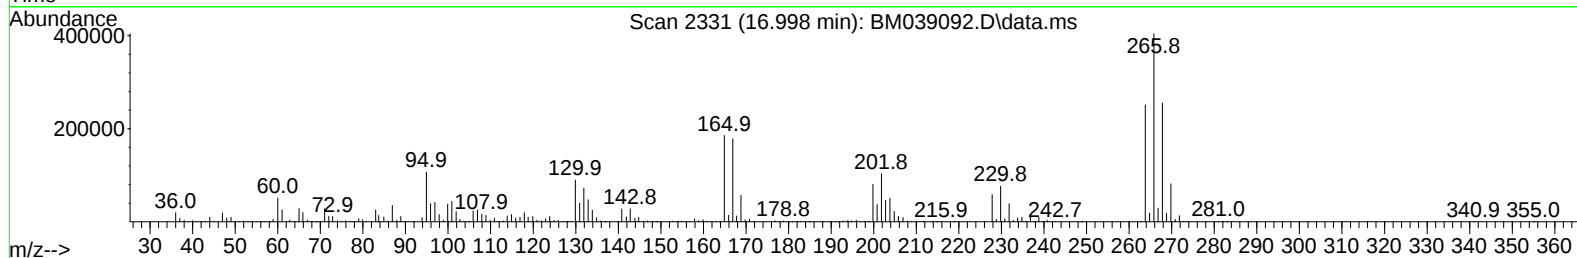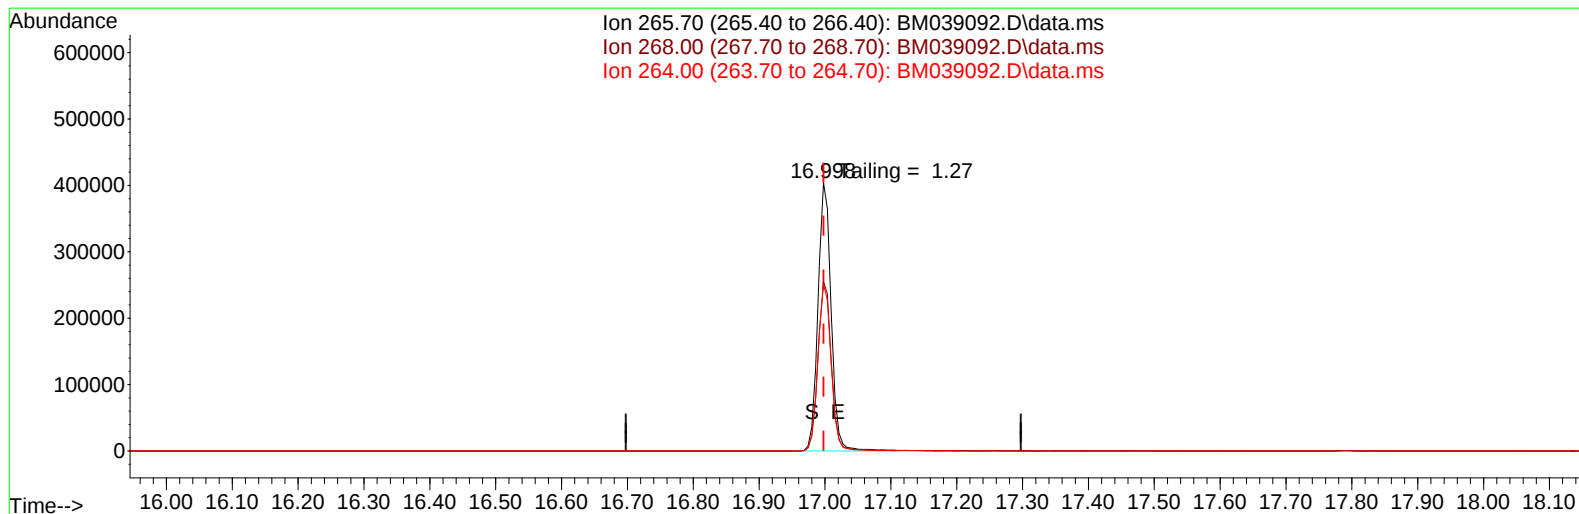

TIC: BM039092.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 150758.07 ng




response 562320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.14
264.00	62.90	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032223\
Data File : BM039092.D
Acq On : 22 Mar 2023 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 23 06:53:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 03:36:20 2023
Response via : Initial Calibration

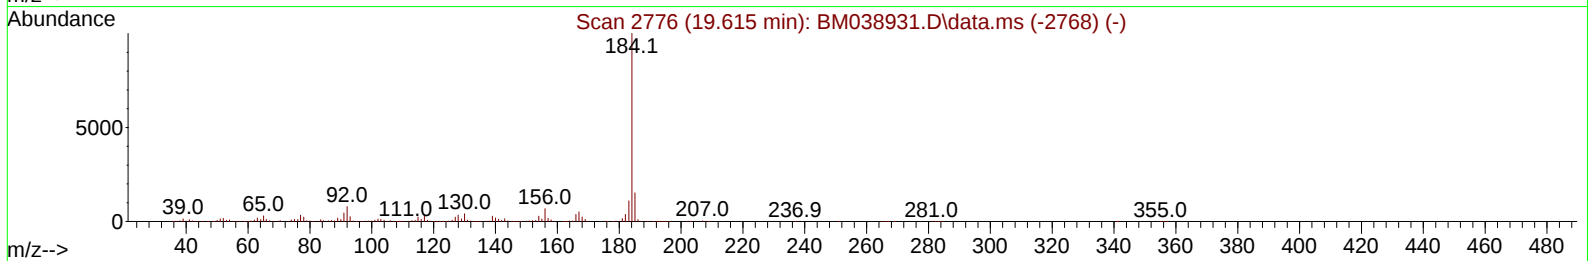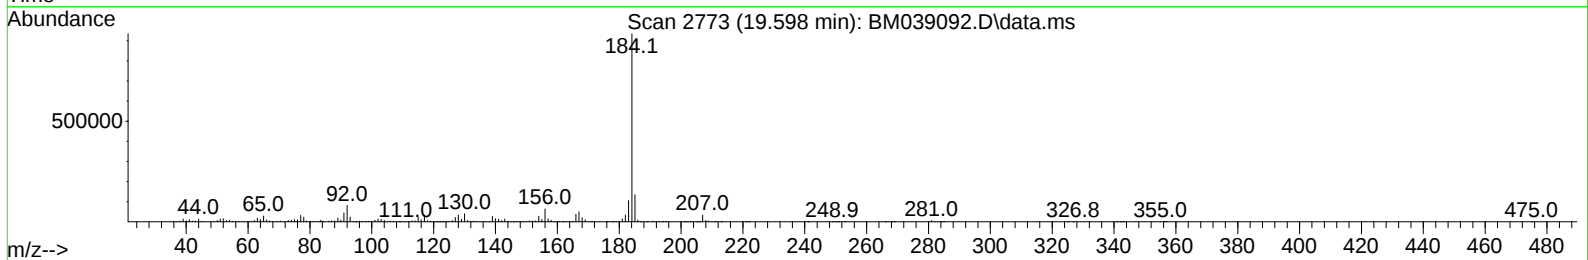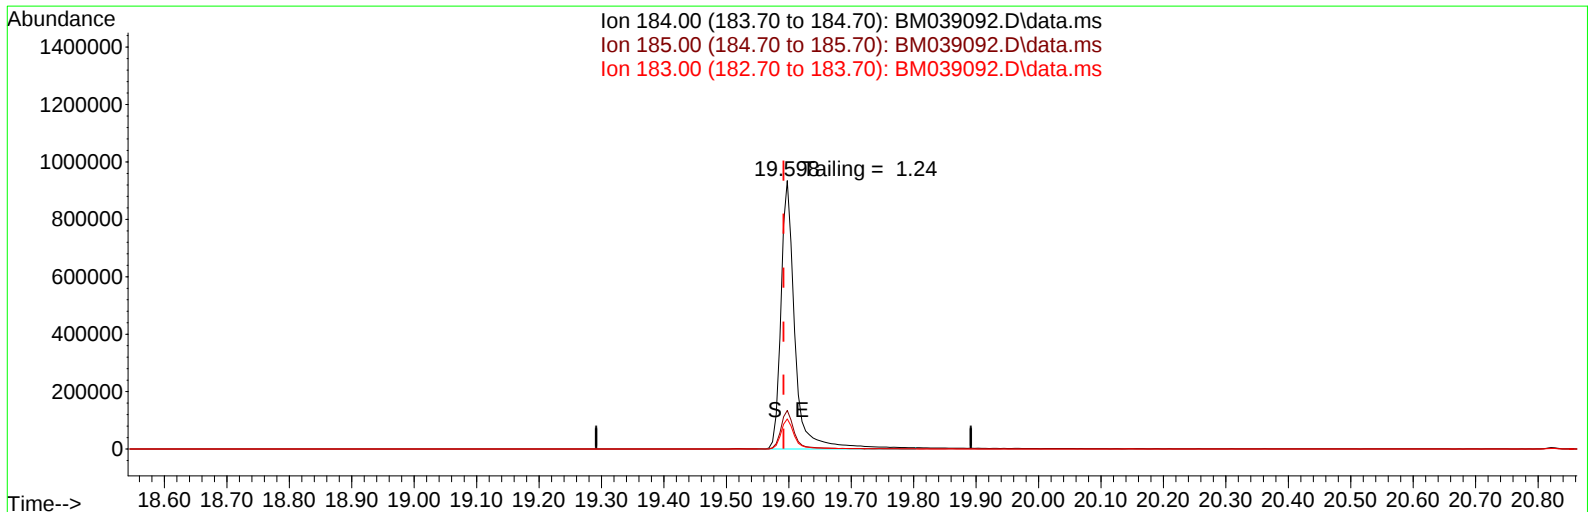

TIC: BM039092.D\data.ms

(77) Benzidine

19.598min (+ 0.006) 7919.72 ng

response 1475781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.40
183.00	11.00	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2023	BNA_M	<u>BM039092.D</u>
Compound Name	Response	Retention Time
DDT	1186412	20.821
DDD	31146	20.386
DDE	888	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32034	1218446	2.63

Instrument :
BNA_M
ClientSampleId :
DFTPP