

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
 Data File : BM019352.D
 Acq On : 23 Mar 2019 15:11
 Operator : JU/SJ
 Sample : K2027-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C09D2

Quant Time: Mar 24 04:56:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 24 04:53:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	131351	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	551679	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	301925	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	673071	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	725042	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	809497	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	13656	4.07	ng/uL	0.00
5) Phenol-d5	6.80	99	57984	4.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	164698	21.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	157971	17.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	98976	11.27	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	83603	21.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	92306	21.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	2169	0.26	ng/ul	0.14
29) 4-Chloroaniline-d4	10.63	131	3013	0.30	ng/ul	0.07
44) Dimethylphthalate-d6	13.69	166	578788	23.76	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	682106	22.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.57	143	2914	0.76	ng/ul	0.06
58) Fluorene-d10	15.27	176	505763	24.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	69838	15.69	ng/ul	0.00
71) Anthracene-d10	17.13	188	823918	25.51	ng/ul	0.00
79) Pyrene-d10	19.43	212	920633	27.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1048789	24.44	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	29620	1.212	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
Data File : BM019352.D
Acq On : 23 Mar 2019 15:11
Operator : JU/SJ
Sample : K2027-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C09D2

Quant Time: Mar 24 04:56:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 24 04:53:47 2019
Response via : Initial Calibration

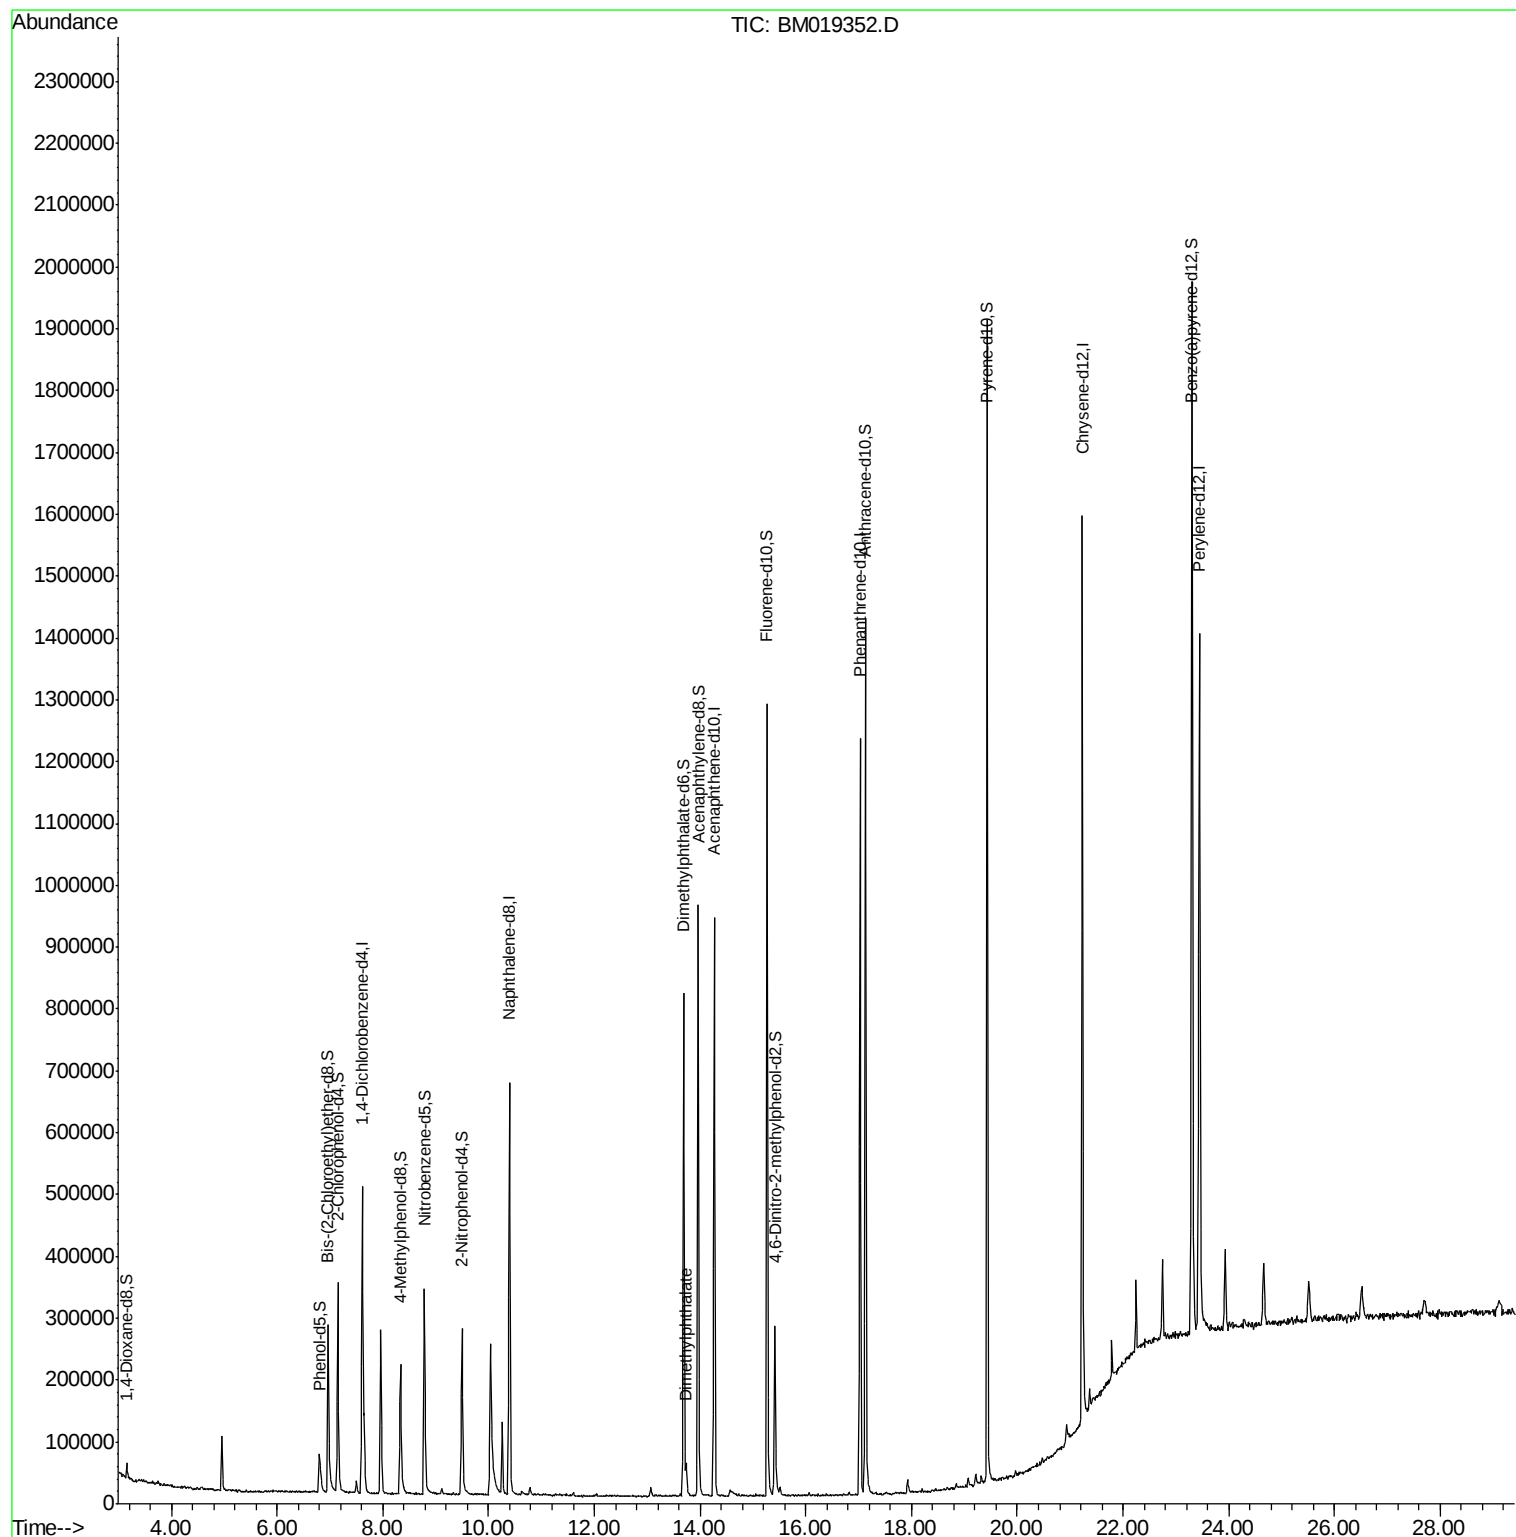

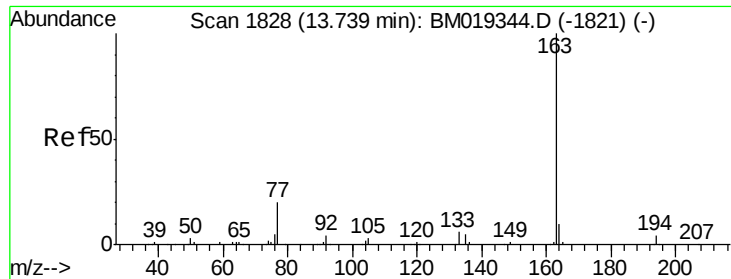

#45

Dimethylphthalate

Concen: 1.212 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BM019352.D


Acq: 23 Mar 2019 15:11

Instrument :

BNA_M

ClientSampleId :

C09D2

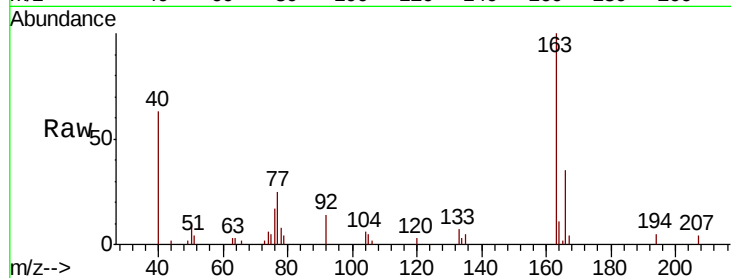

Tgt Ion:	163	Resp:	29620
Ion	Ratio	Lower	Upper
163	100		
194	5.1	4.0	6.0
164	11.5	8.4	12.6

