

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
 Data File : BM019357.D
 Acq On : 23 Mar 2019 18:11
 Operator : JU/SJ
 Sample : K1968-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C09E9

Quant Time: Mar 24 04:57:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 24 04:53:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	132510	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	557338	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	318704	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	705883	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	741927	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	841710	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	14539	4.30	ng/uL	0.00
5) Phenol-d5	6.80	99	71200	6.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	241116	30.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	236750	26.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	138900	15.68	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	135522	34.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	155951	35.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	254268	30.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	2575	0.26	ng/ul	0.05
44) Dimethylphthalate-d6	13.69	166	946694	36.81	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1161967	36.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	9460	2.35	ng/ul	0.04
58) Fluorene-d10	15.27	176	823010	37.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	130719	28.00	ng/ul	0.00
71) Anthracene-d10	17.13	188	1272746	37.57	ng/ul	0.00
79) Pyrene-d10	19.43	212	1395889	40.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	1601388	35.89	ng/ul	-0.01

Target Compounds


					Qvalue	
37) 1,2,4,5-Tetrachlorobenzene	12.41	216	31336	3.090	ng/ul#	89
73) 1,2,3,4-Tetrachlorobenzene	13.06	216	30662	2.996	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
Data File : BM019357.D
Acq On : 23 Mar 2019 18:11
Operator : JU/SJ
Sample : K1968-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C09E9

Quant Time: Mar 24 04:57:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 24 04:53:47 2019
Response via : Initial Calibration




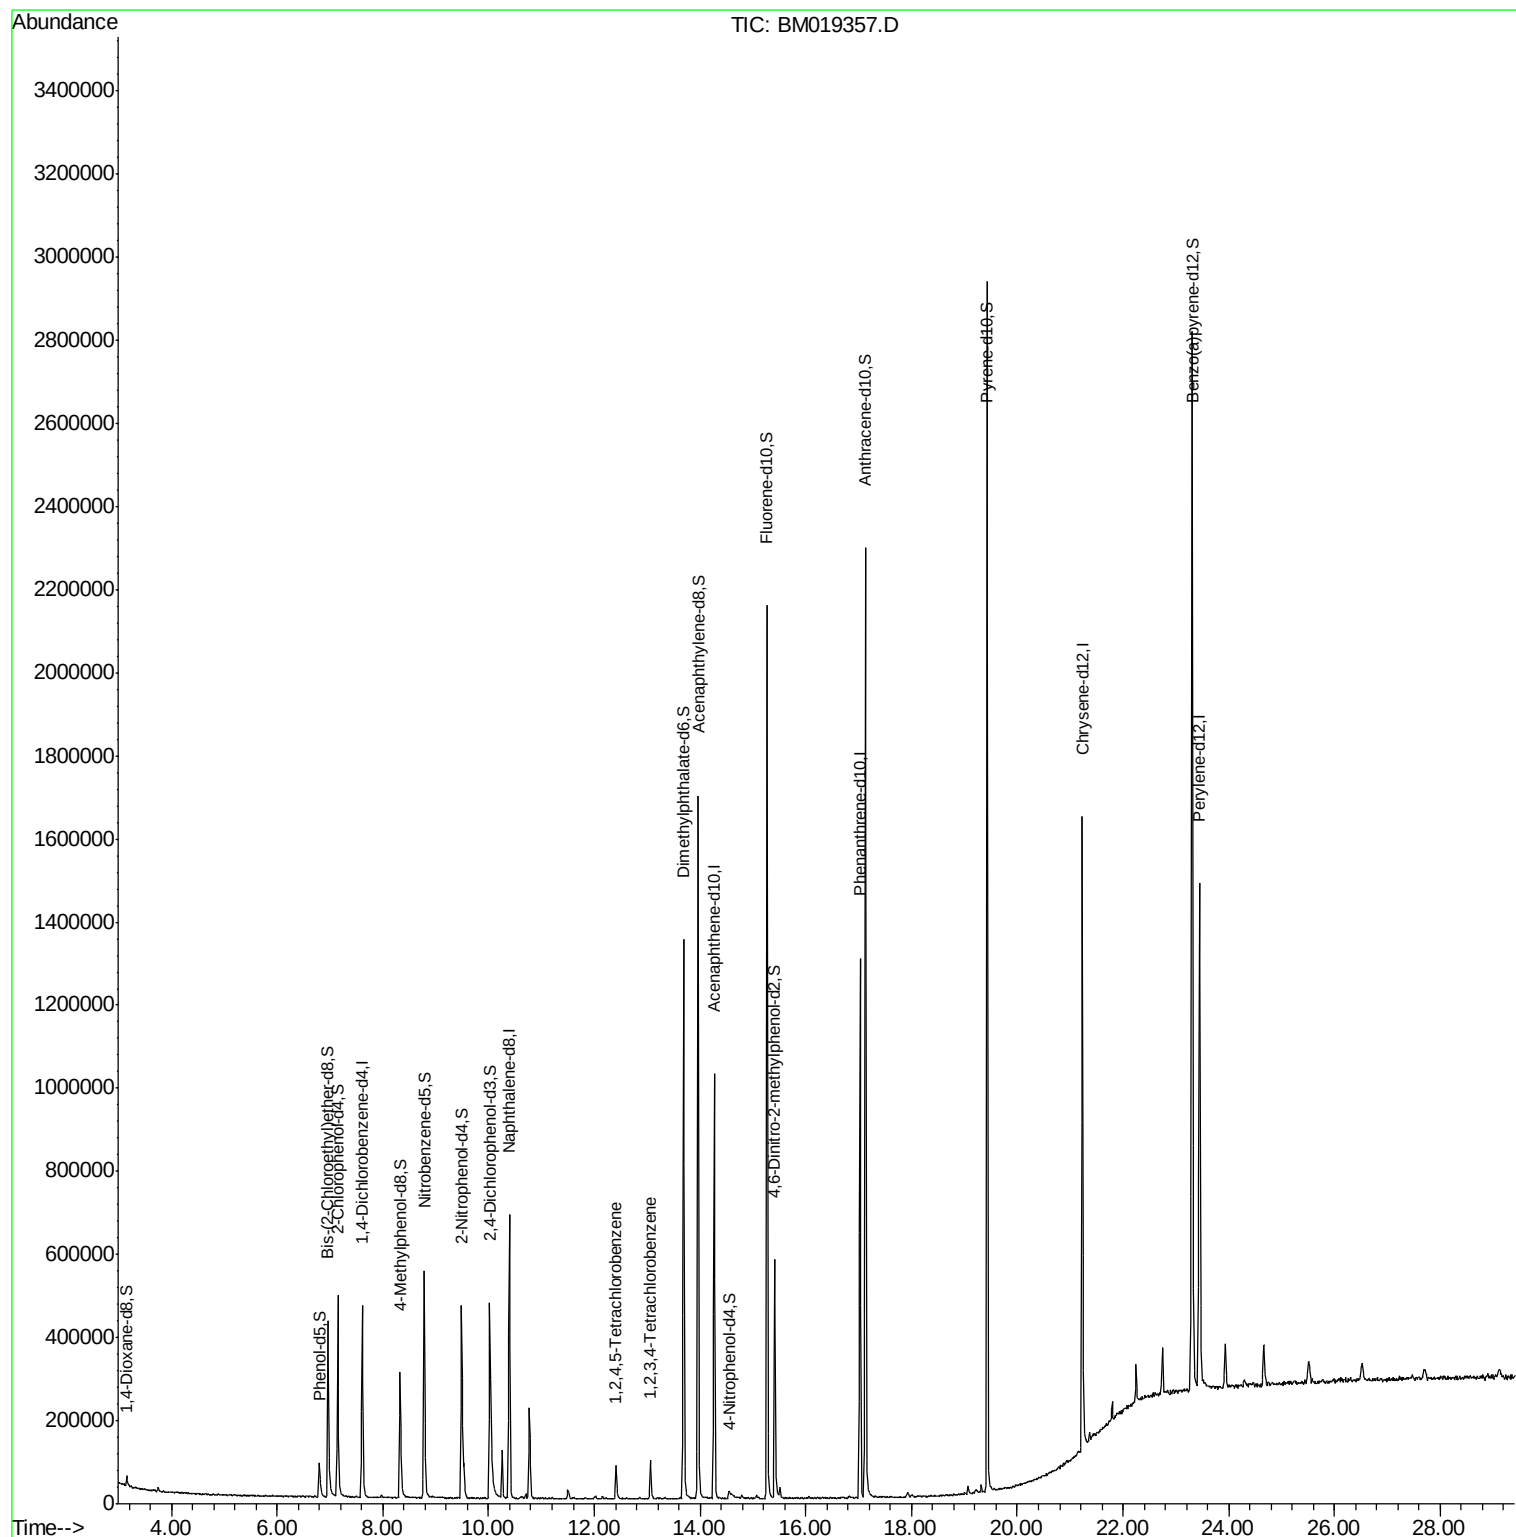


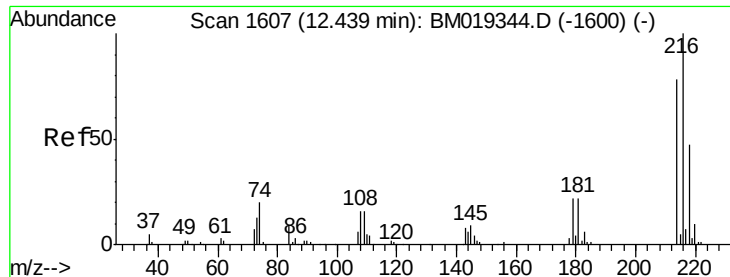

#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 3.090 ng/uL
 RT: 12.41 min Scan# 1602
 Delta R.T. -0.03 min
 Lab File: BM019357.D
 Acq: 23 Mar 2019 18:11

Instrument :
 BNA_M
 ClientSampleId :
 C09E9

Tgt Ion:216 Resp: 31336
 Ion Ratio Lower Upper
 216 100
 214 88.0 64.1 96.1
 179 24.0 14.5 21.7#
 108 20.9 10.4 15.6#

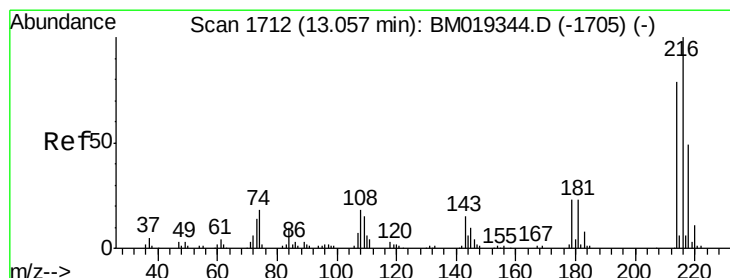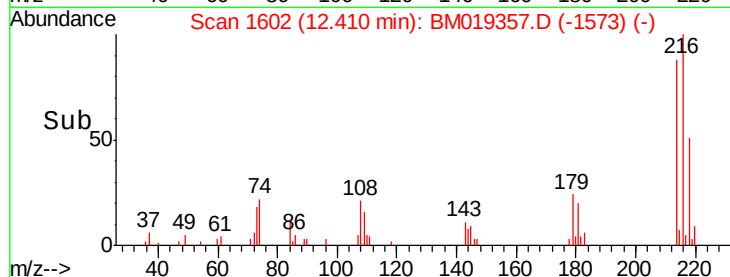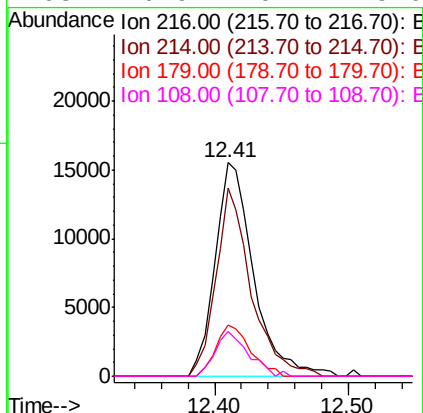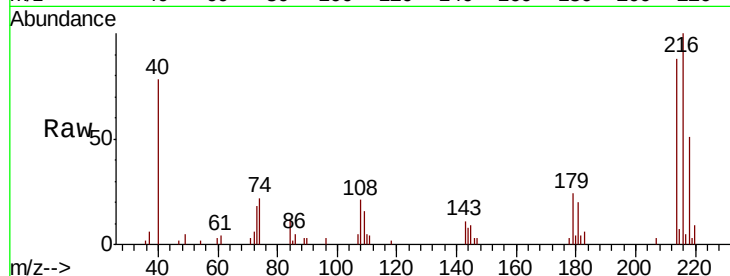

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 2.996 ng/uL
 RT: 13.06 min Scan# 1713
 Delta R.T. 0.01 min
 Lab File: BM019357.D
 Acq: 23 Mar 2019 18:11

Tgt Ion:216 Resp: 30662
 Ion Ratio Lower Upper
 216 100
 214 76.7 64.1 96.1
 218 47.7 39.4 59.0

