

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
 Data File : BM019359.D
 Acq On : 23 Mar 2019 19:23
 Operator : JU/SJ
 Sample : PB118136BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK36

Quant Time: Mar 24 04:57:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 24 04:53:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	126599	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	549009	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	314172	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	699819	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	745301	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	846532	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	22243	6.88	ng/uL	0.00
5) Phenol-d5	6.79	99	380682	33.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	249513	33.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	298870	34.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	308078	36.41	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	142582	36.41	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	159692	36.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	265106	32.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	409572	41.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1076668	42.47	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1241967	39.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	130334	32.80	ng/ul	0.00
58) Fluorene-d10	15.27	176	889771	40.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	134160	28.99	ng/ul	0.00
71) Anthracene-d10	17.13	188	1425410	42.44	ng/ul	0.00
79) Pyrene-d10	19.43	212	1558986	45.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	1829565	40.77	ng/ul	-0.01

Target Compounds


					Qvalue	
15) N-Nitroso-di-n-propylamine	8.32	70	8419	1.090	ng/ul#	1
46) 2,6-Dinitrotoluene	13.69	165	6601	1.414	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
Data File : BM019359.D
Acq On : 23 Mar 2019 19:23
Operator : JU/SJ
Sample : PB118136BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Quant Time: Mar 24 04:57:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 24 04:53:47 2019
Response via : Initial Calibration




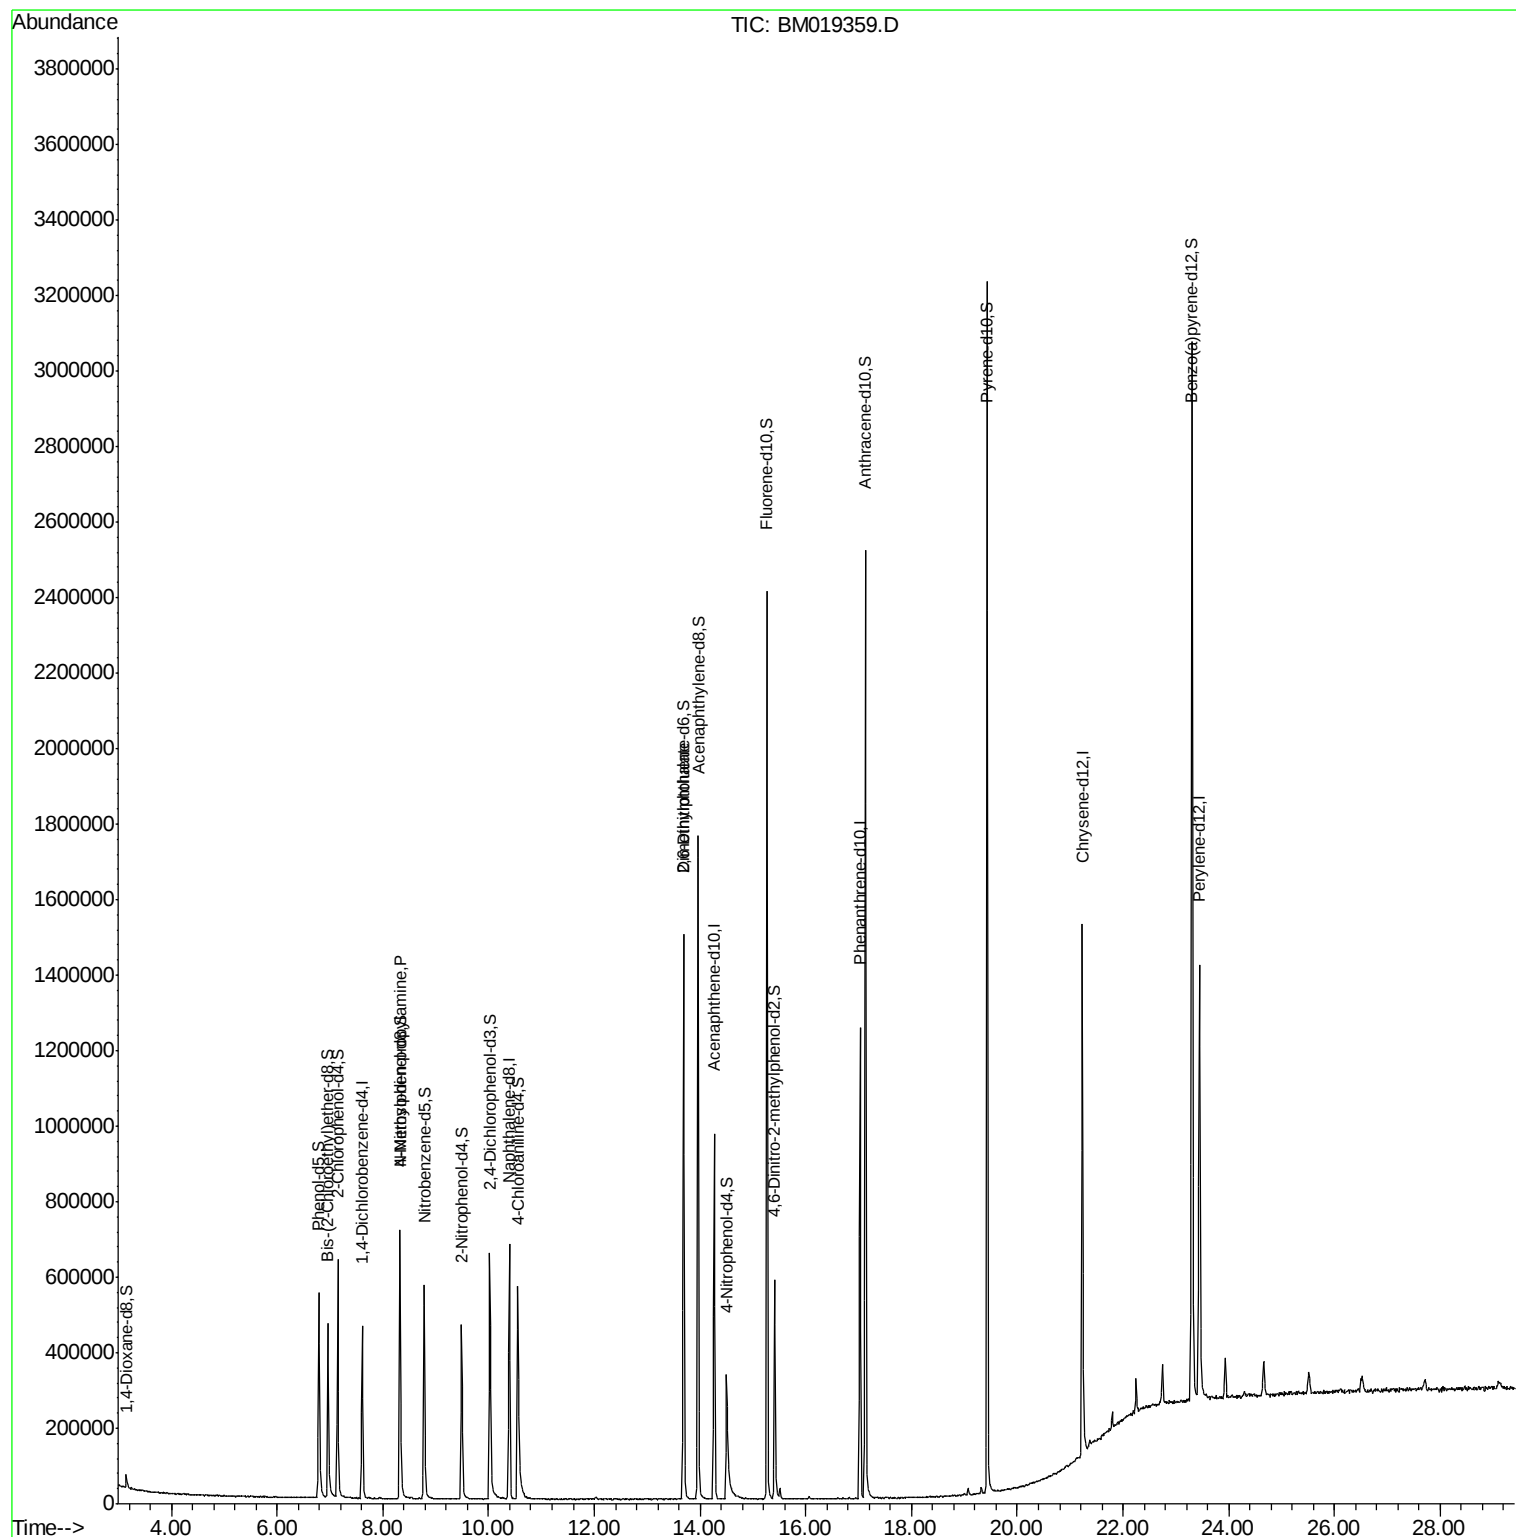


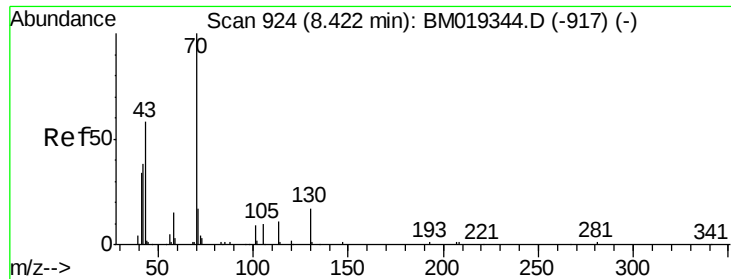

#15
N-Nitroso-di-n-propylamine
Concen: 1.090 ng/ul
RT: 8.32 min Scan# 907
Delta R.T. -0.11 min
Lab File: BM019359.D
Acq: 23 Mar 2019 19:23

Instrument :
BNA_M
ClientSampleId :
SBLK36

Tgt Ion:	70	Resp:	8419
Ion	Ratio	Lower	Upper
70	100		
42	259.1	40.2	60.4#
101	0.0	7.7	11.5#
130	0.0	17.8	26.6#

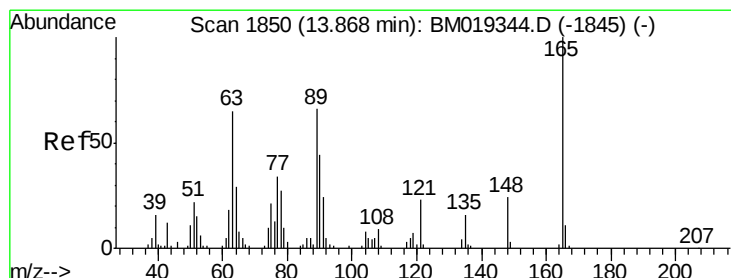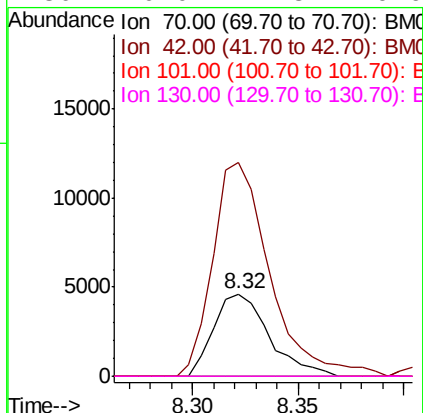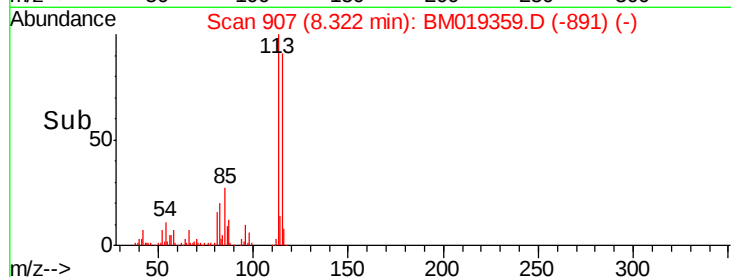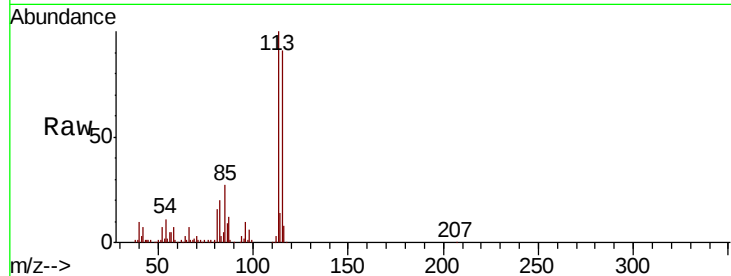

#46
2,6-Dinitrotoluene
Concen: 1.414 ng/ul
RT: 13.69 min Scan# 1820
Delta R.T. -0.18 min
Lab File: BM019359.D
Acq: 23 Mar 2019 19:23

Tgt Ion:	165	Resp:	6601
Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.8	65.8#
121	25.8	17.8	26.6

