

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
 Data File : BM019379.D
 Acq On : 24 Mar 2019 07:24
 Operator : JU/SJ
 Sample : K2031-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5W1

Quant Time: Mar 25 02:06:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 02:03:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	141528	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	606579	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.27	164	342206	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	773889	20.00	ng/ul	-0.01
78) Chrysene-d12	21.23	240	862010	20.00	ng/ul	-0.01
86) Perylene-d12	23.44	264	967334	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	20679	5.72	ng/uL	0.00
5) Phenol-d5	6.79	99	181197	14.38	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.96	67	138805	16.45	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.14	132	159723	16.72	ng/ul	-0.01
13) 4-Methylphenol-d8	8.32	113	157241	16.62	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	71698	16.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	78721	16.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	138296	15.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	177258	16.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	557477	20.19	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	606587	17.57	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.53	143	17912	4.14	ng/ul	0.02
58) Fluorene-d10	15.27	176	472092	19.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	39970	7.81	ng/ul	0.00
71) Anthracene-d10	17.12	188	721210	19.42	ng/ul	-0.01
79) Pyrene-d10	19.43	212	806158	20.25	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.30	264	930202	18.14	ng/ul	-0.02


Target Compounds				Qvalue		
6) Phenol	6.82	94	19754	1.502	ng/ul#	86
45) Dimethylphthalate	13.73	163	111047	4.008	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
Data File : BM019379.D
Acq On : 24 Mar 2019 07:24
Operator : JU/SJ
Sample : K2031-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5W1

Quant Time: Mar 25 02:06:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 02:03:45 2019
Response via : Initial Calibration

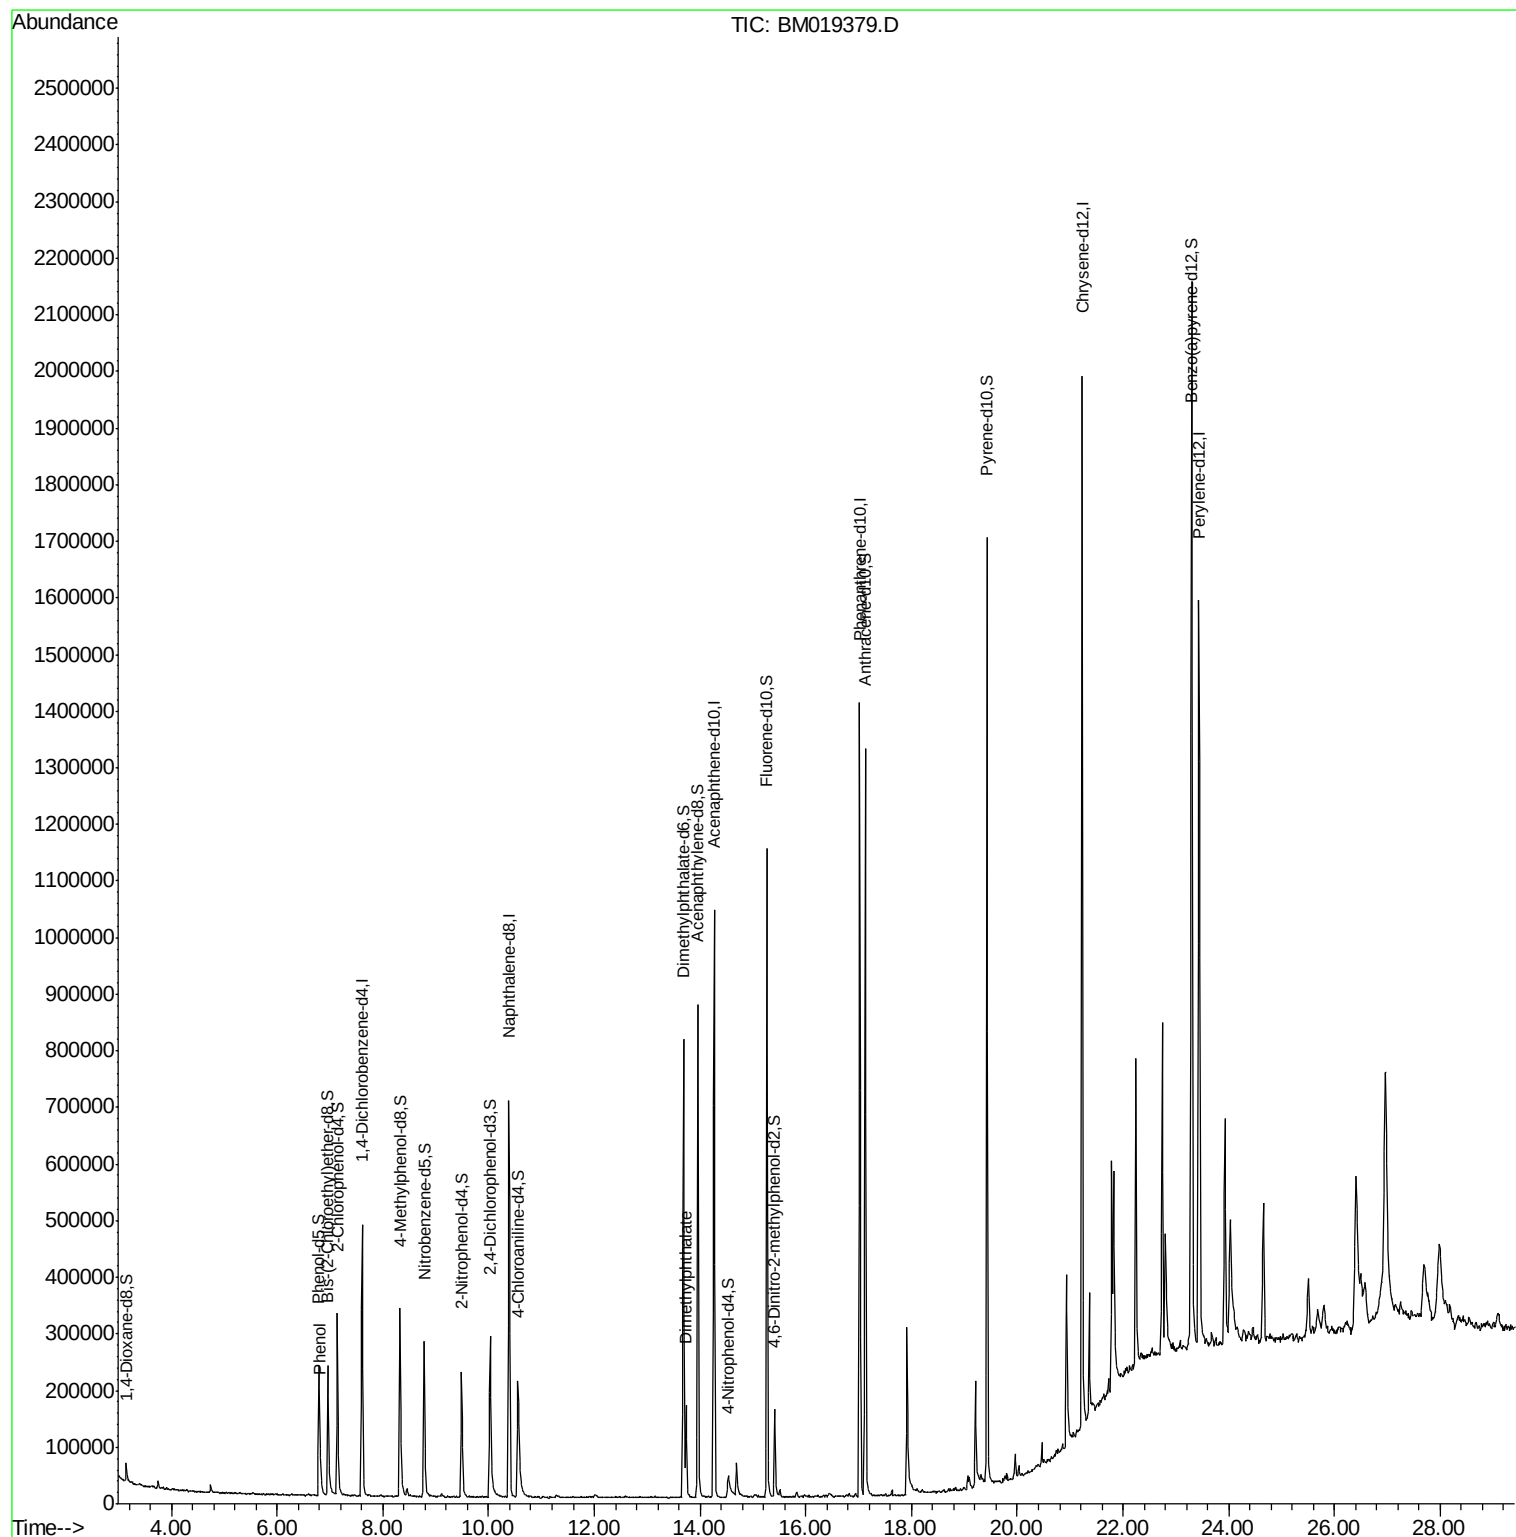

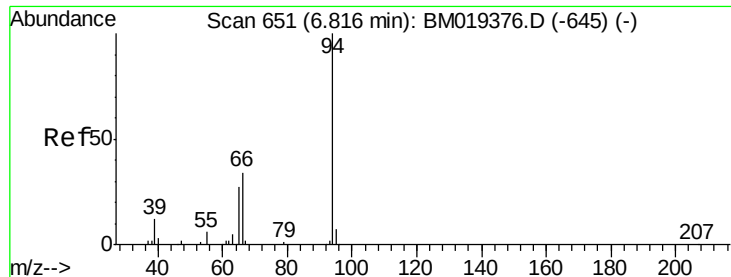





#6

Phenol

Concen: 1.502 ng/ul
 RT: 6.82 min Scan# 651
 Delta R.T. -0.01 min
 Lab File: BM019379.D
 Acq: 24 Mar 2019 07:24

Instrument :
 BNA_M
 ClientSampleId :
 BF5W1

Tgt Ion: 94 Resp: 19754
 Ion Ratio Lower Upper
 94 100
 65 31.9 23.0 34.6
 66 49.6 30.4 45.6#

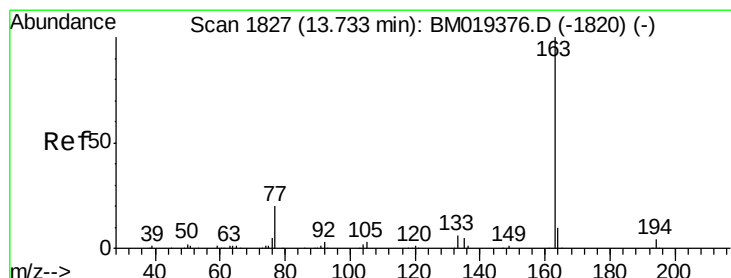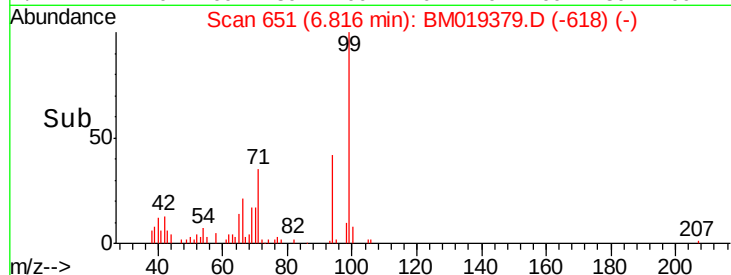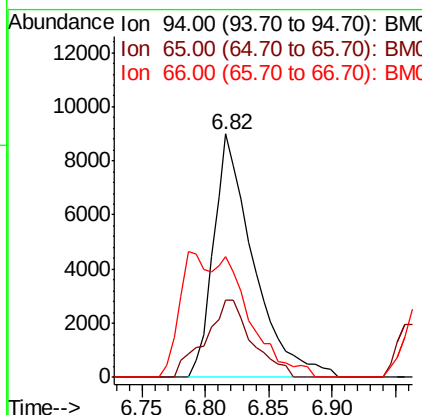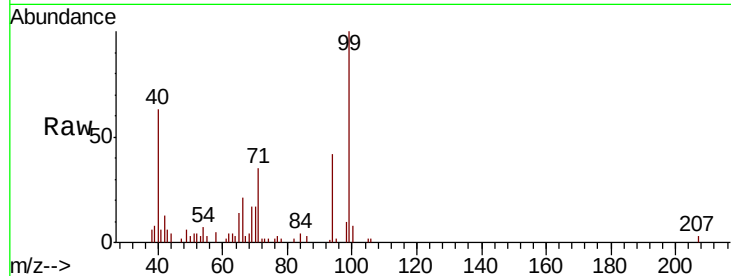

#45

Dimethylphthalate

Concen: 4.008 ng/ul
 RT: 13.73 min Scan# 1827
 Delta R.T. -0.01 min
 Lab File: BM019379.D
 Acq: 24 Mar 2019 07:24

Tgt Ion: 163 Resp: 111047
 Ion Ratio Lower Upper
 163 100
 194 4.3 4.0 6.0
 164 9.3 8.4 12.6

