

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
 Data File : BM019348.D
 Acq On : 23 Mar 2019 12:45
 Operator : JU/SJ
 Sample : K2027-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0992

Manual Integrations
 APPROVED

Sohil
 3/26/2019 6:25:27 PM

Quant Time: Mar 24 05:29:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 24 04:53:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	123272	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	521289	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	301461	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	675373	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	731310	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	821838	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	12865	4.09	ng/uL	0.00
5) Phenol-d5	6.80	99	65051	5.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	209430	28.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	194852	23.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	118741	14.41	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	110158	29.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	122258	29.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	205587m	26.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	1543	0.16	ng/ul	0.05
44) Dimethylphthalate-d6	13.69	166	785081	32.28	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	927232	30.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	12413m	3.26	ng/ul	0.04
58) Fluorene-d10	15.27	176	670528	32.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	101329	22.69	ng/ul	0.00
71) Anthracene-d10	17.13	188	1077294	33.24	ng/ul	0.00
79) Pyrene-d10	19.43	212	1177966	34.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	1384354	31.77	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
33) 4-Chloro-3-methylphenol	11.73	107	26864m	3.230	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
Data File : BM019348.D
Acq On : 23 Mar 2019 12:45
Operator : JU/SJ
Sample : K2027-03
Misc :
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
C0992

Quant Time: Mar 24 05:29:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 24 04:53:47 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/26/2019 6:25:27 PM

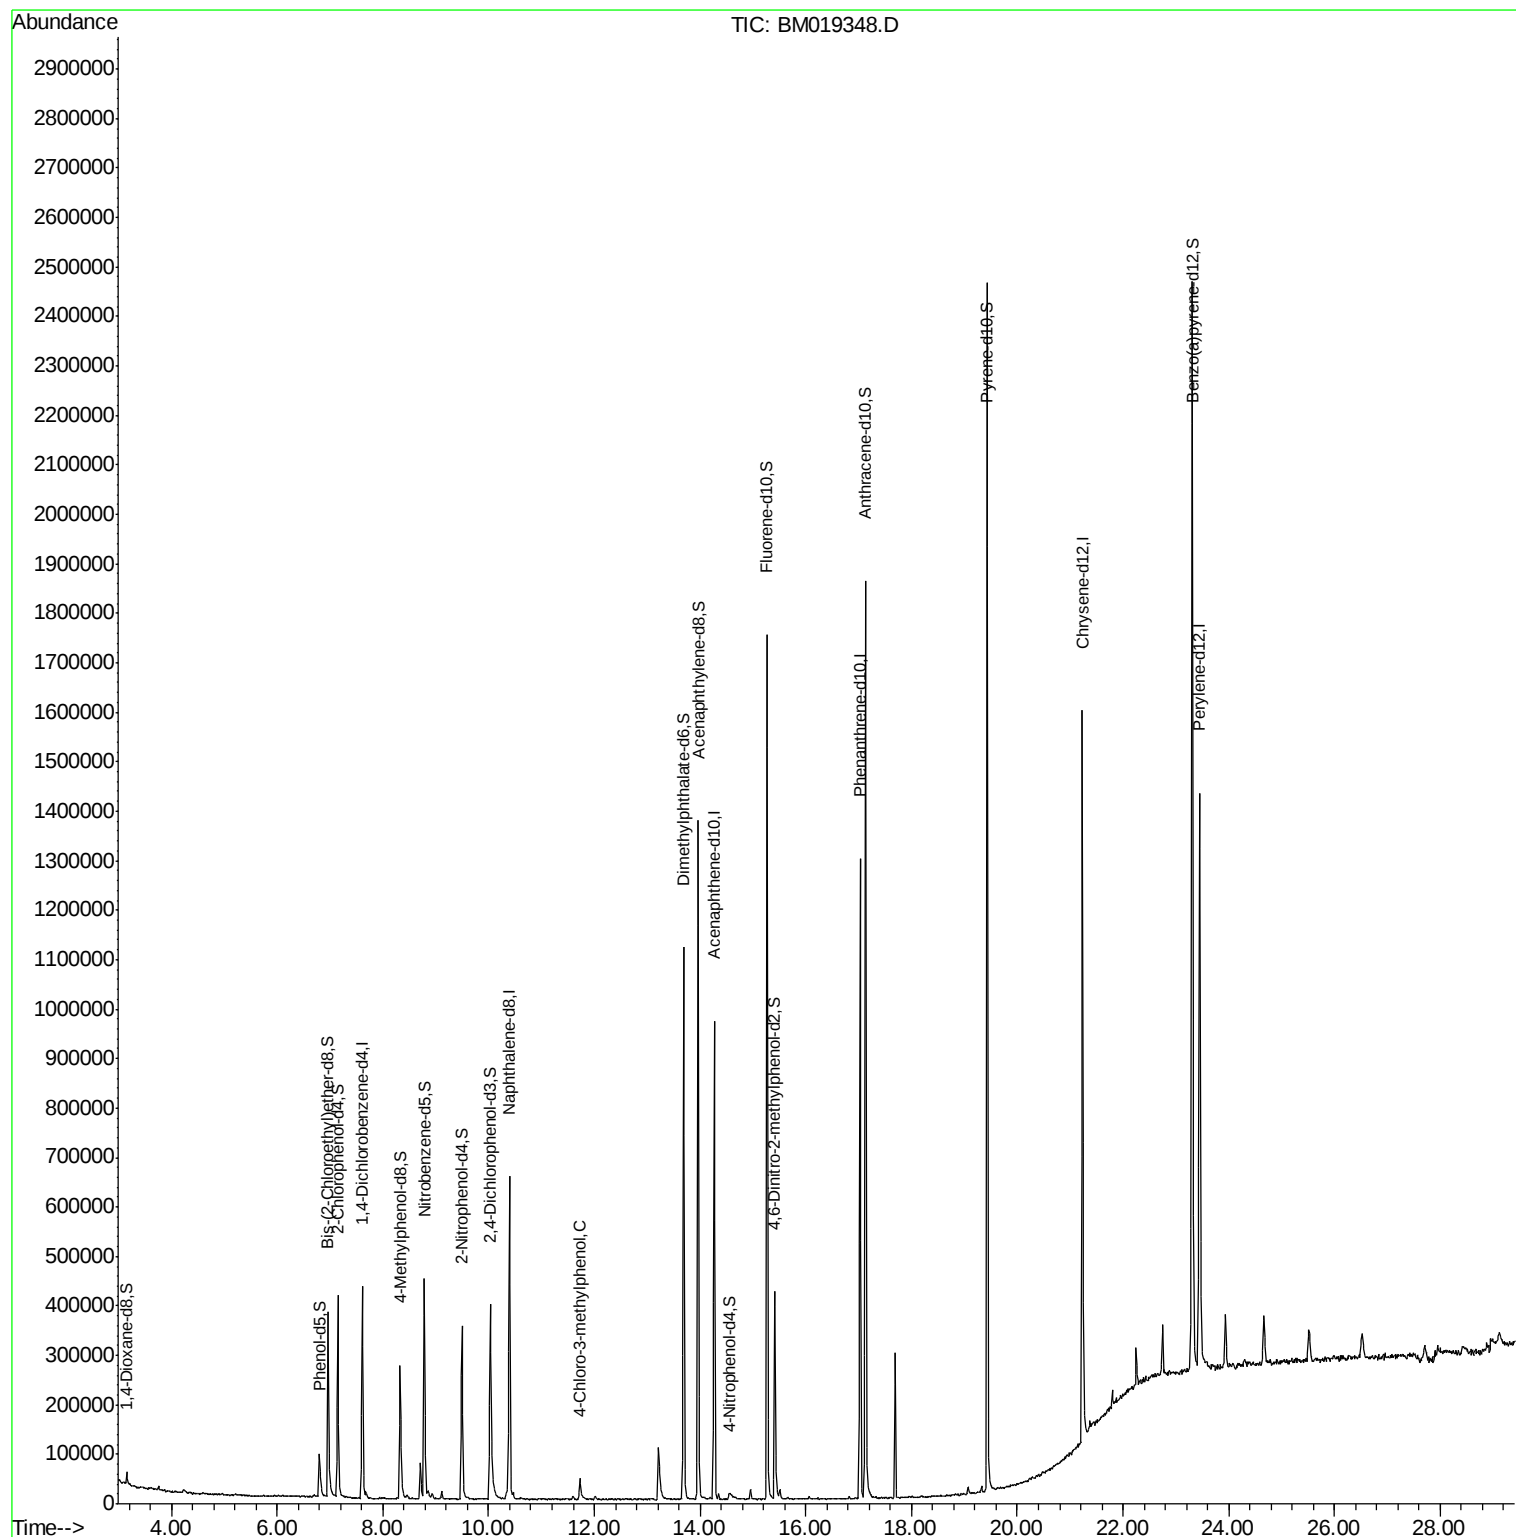

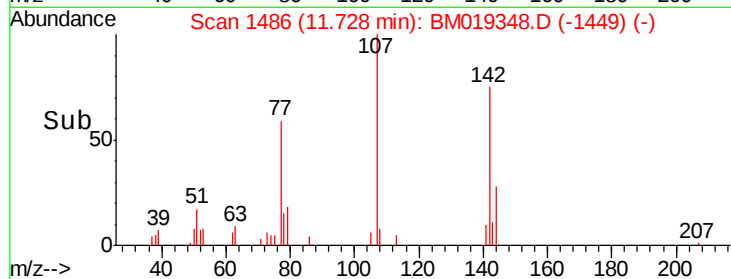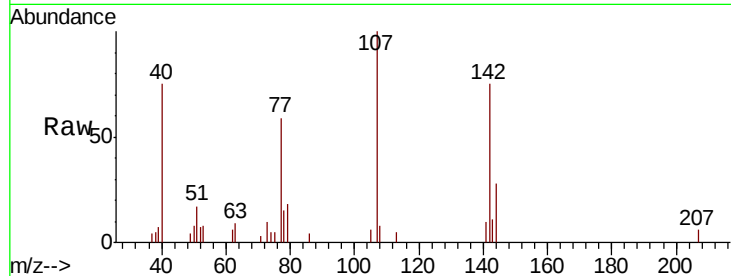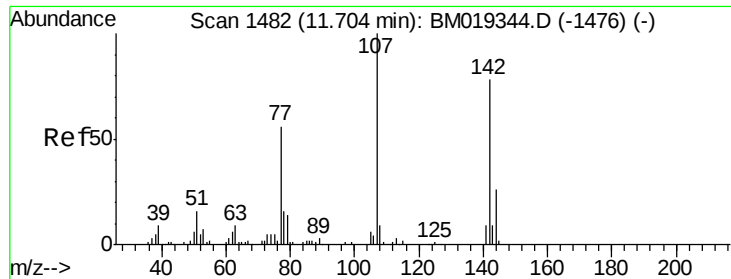

#33

4-Chloro-3-methylphenol

Concen: 3.230 ng/ul m

RT: 11.73 min Scan# 1486

Delta R.T. 0.02 min

Lab File: BM019348.D

Acq: 23 Mar 2019 12:45

Instrument :

BNA_M

ClientSampleId :

C0992

Tot Ion:	107	Resp:	26864
Ion Ratio	Lower	Upper	
107	100		
144	28.0	21.1	31.7
142	74.9	60.1	90.1

Manual Integrations
APPROVED

Sohil
3/26/2019 6:25:27 PM

