

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
 Data File : BM019368.D
 Acq On : 24 Mar 2019 00:47
 Operator : JU/SJ
 Sample : K2031-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5Y0

Manual Integrations
 APPROVED

Sohil
 3/26/2019 6:25:46 PM

Quant Time: Mar 25 01:16:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 00:34:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	140697	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	595016	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	345936	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	807702	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	911302	20.00	ng/ul	-0.01
86) Perylene-d12	23.44	264	1017590	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	15737	4.38	ng/uL	0.00
5) Phenol-d5	6.79	99	90801	7.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	237315	28.29	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.15	132	247391	26.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	161564	17.18	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	133369	31.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	151396	32.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	269341	30.22	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.69	166	977029	35.00	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1132353	32.44	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.54	143	22405m	5.12	ng/ul	0.03
58) Fluorene-d10	15.27	176	830022	34.51	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	153014	28.65	ng/ul	0.00
71) Anthracene-d10	17.12	188	1381351	35.64	ng/ul	-0.01
79) Pyrene-d10	19.43	212	1571000	37.32	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.30	264	1821332	33.76	ng/ul	-0.02

Target Compounds					Ovalue	
33) 4-Chloro-3-methylphenol	11.72	107	23652	2.491	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
Data File : BM019368.D
Acq On : 24 Mar 2019 00:47
Operator : JU/SJ
Sample : K2031-13
Misc :
ALS Vial : 26 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BF5Y0

Quant Time: Mar 25 01:16:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 00:34:42 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/26/2019 6:25:46 PM

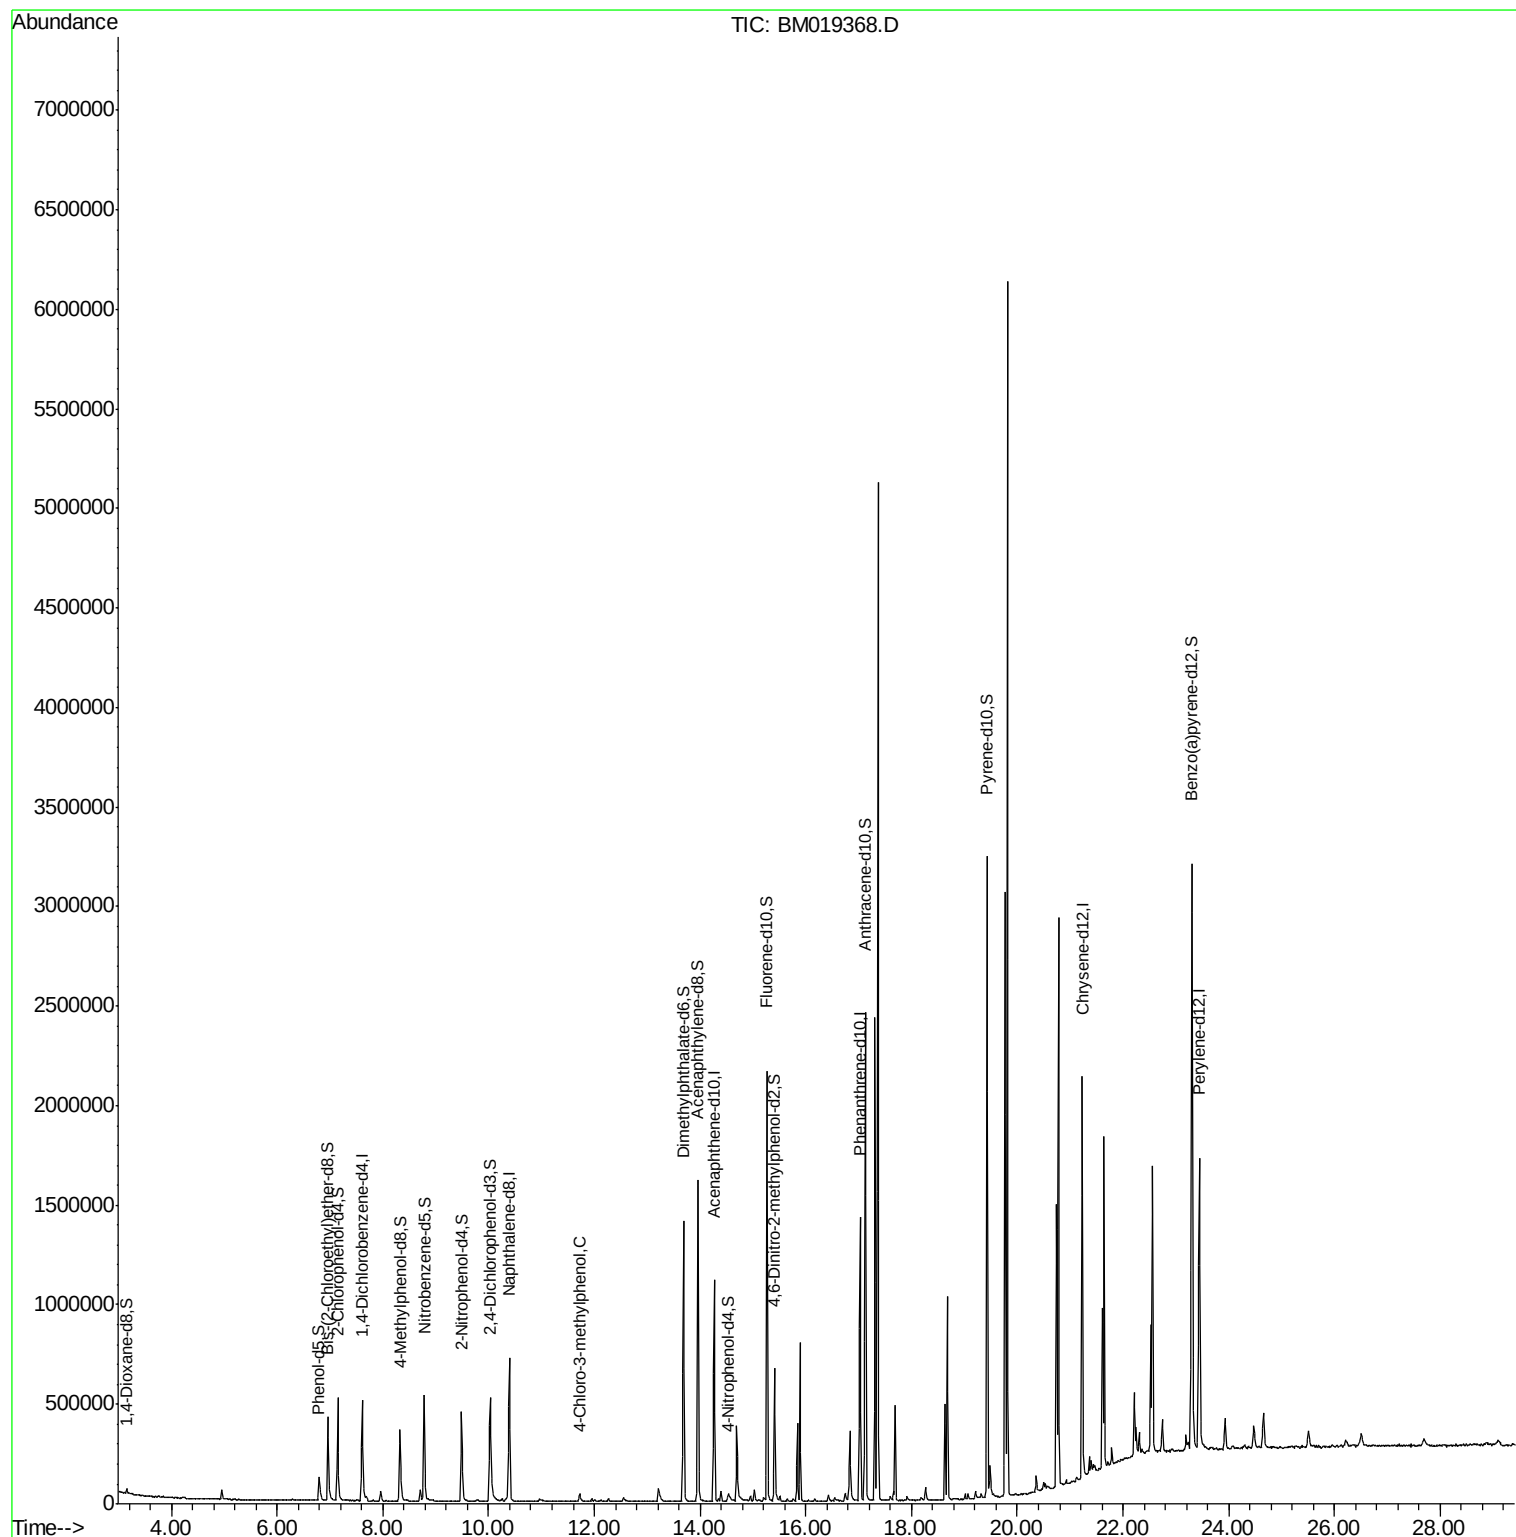

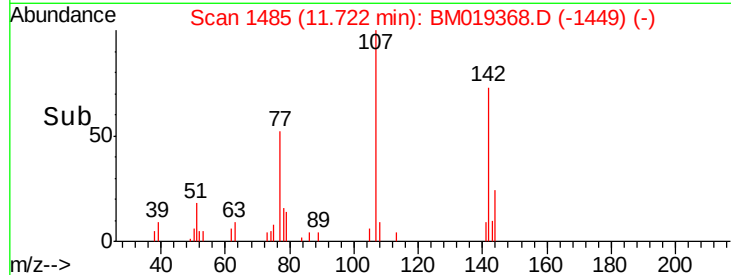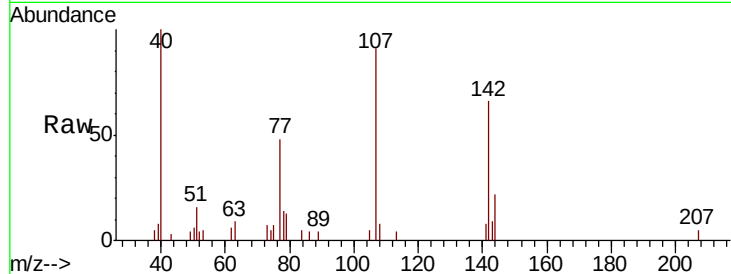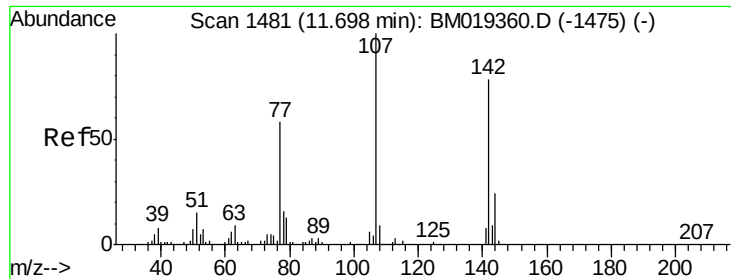

#33
 4-Chloro-3-methylphenol
 Concen: 2.491 ng/ul
 RT: 11.72 min Scan# 1485
 Delta R.T. 0.01 min
 Lab File: BM019368.D
 Acq: 24 Mar 2019 00:47

Instrument :
 BNA_M
 ClientSampleId :
 BF5Y0

Tot Ion	Ratio	Lower	Upper
107	100		
144	24.0	21.1	31.7
142	72.6	60.1	90.1

Manual Integrations
 APPROVED

Sohil
 3/26/2019 6:25:46 PM

