

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
 Data File : BM019354.D
 Acq On : 23 Mar 2019 16:23
 Operator : JU/SJ
 Sample : K2025-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0982

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	35	rVB2	24643	32134	0.83%	0.101%
2	4.963	332	336	339	rBV3	4280	6829	0.18%	0.022%
3	5.322	394	397	400	rBV3	3165	4171	0.11%	0.013%
4	6.798	643	648	660	rBV2	63259	153298	3.98%	0.484%
5	6.963	670	676	699	rBV	315506	607668	15.78%	1.917%
6	7.145	701	707	720	rBV	379350	662472	17.20%	2.090%
7	7.610	780	786	802	rBV	475133	807146	20.96%	2.546%
8	7.963	843	846	851	rVB4	5138	8169	0.21%	0.026%
9	8.328	902	908	923	rBV	217178	434646	11.29%	1.371%
10	8.781	978	985	998	rBV	380233	690994	17.94%	2.180%
11	9.116	1035	1042	1053	rVB2	19707	31825	0.83%	0.100%
12	9.498	1100	1107	1125	rBV	304193	574219	14.91%	1.812%
13	10.034	1190	1198	1219	rBV	285117	793902	20.61%	2.505%
14	10.392	1252	1259	1275	rVV	689749	1184131	30.75%	3.736%
15	10.633	1294	1300	1306	rBV4	3752	9928	0.26%	0.031%
16	11.598	1455	1464	1469	rBV2	17618	26993	0.70%	0.085%
17	12.045	1536	1540	1544	rVB3	2630	4143	0.11%	0.013%
18	12.169	1556	1561	1562	rBV2	2439	3897	0.10%	0.012%
19	12.616	1633	1637	1640	rVB3	2215	4251	0.11%	0.013%
20	13.098	1713	1719	1725	rVB4	13225	20210	0.52%	0.064%
21	13.298	1747	1753	1758	rBV4	7455	12415	0.32%	0.039%
22	13.686	1814	1819	1838	rBV	967879	1552209	40.30%	4.897%
23	13.963	1859	1866	1877	rBV	1237622	1803629	46.83%	5.690%
24	14.269	1912	1918	1930	rBV2	1082813	1613182	41.89%	5.089%
25	14.557	1963	1967	1970	rBV4	11149	20902	0.54%	0.066%
26	14.592	1970	1973	1979	rVB5	9171	17480	0.45%	0.055%
27	15.268	2082	2088	2105	rBV	1597750	2418951	62.81%	7.631%
28	15.410	2107	2112	2124	rVV	387135	648935	16.85%	2.047%
29	15.515	2127	2130	2136	rVV	19816	29052	0.75%	0.092%
30	16.057	2219	2222	2227	rVB3	4828	5828	0.15%	0.018%
31	16.815	2349	2351	2355	rVB4	4787	5662	0.15%	0.018%
32	17.027	2379	2387	2397	rBV	1384414	1930683	50.13%	6.091%
33	17.127	2397	2404	2422	rVV	1872213	2759325	71.64%	8.705%
34	17.921	2533	2539	2550	rBV3	33272	67528	1.75%	0.213%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
 Data File : BM019354.D
 Acq On : 23 Mar 2019 16:23
 Operator : JU/SJ
 Sample : K2025-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0982

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

35	18.392	2614	2619	2622	rBV5	3424	6144	0.16%	0.019%
36	19.068	2729	2734	2738	rBV2	15660	24696	0.64%	0.078%
37	19.209	2753	2758	2765	rBV2	55036	95195	2.47%	0.300%
38	19.327	2773	2778	2781	rVB	12335	15391	0.40%	0.049%
39	19.433	2790	2796	2809	rBV	2482529	3228587	83.83%	10.186%
40	19.968	2885	2887	2890	rBV3	6275	6412	0.17%	0.020%
41	20.468	2969	2972	2974	rBV3	12492	12515	0.32%	0.039%
42	20.503	2976	2978	2979	rBV2	9354	6911	0.18%	0.022%
43	20.615	2995	2997	2998	rBV2	12056	5727	0.15%	0.018%
44	21.233	3096	3102	3115	rBV	1662807	2374965	61.66%	7.493%
45	21.368	3123	3125	3128	rVB3	39209	36140	0.94%	0.114%
46	21.792	3195	3197	3204	rVB3	66155	83984	2.18%	0.265%
47	22.250	3272	3275	3283	rVB	111606	147315	3.82%	0.465%
48	22.750	3356	3360	3364	rVB	121631	168882	4.38%	0.533%
49	23.303	3448	3454	3466	rVB	2119863	3851429	100.00%	12.150%
50	23.450	3472	3479	3493	rBV	1298828	2486775	64.57%	7.845%
51	23.933	3558	3561	3569	rVB2	108786	199843	5.19%	0.630%


Sum of corrected areas: 31697718

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032319\
Data File : BM019354.D
Acq On : 23 Mar 2019 16:23
Operator : JU/SJ
Sample : K2025-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0982

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

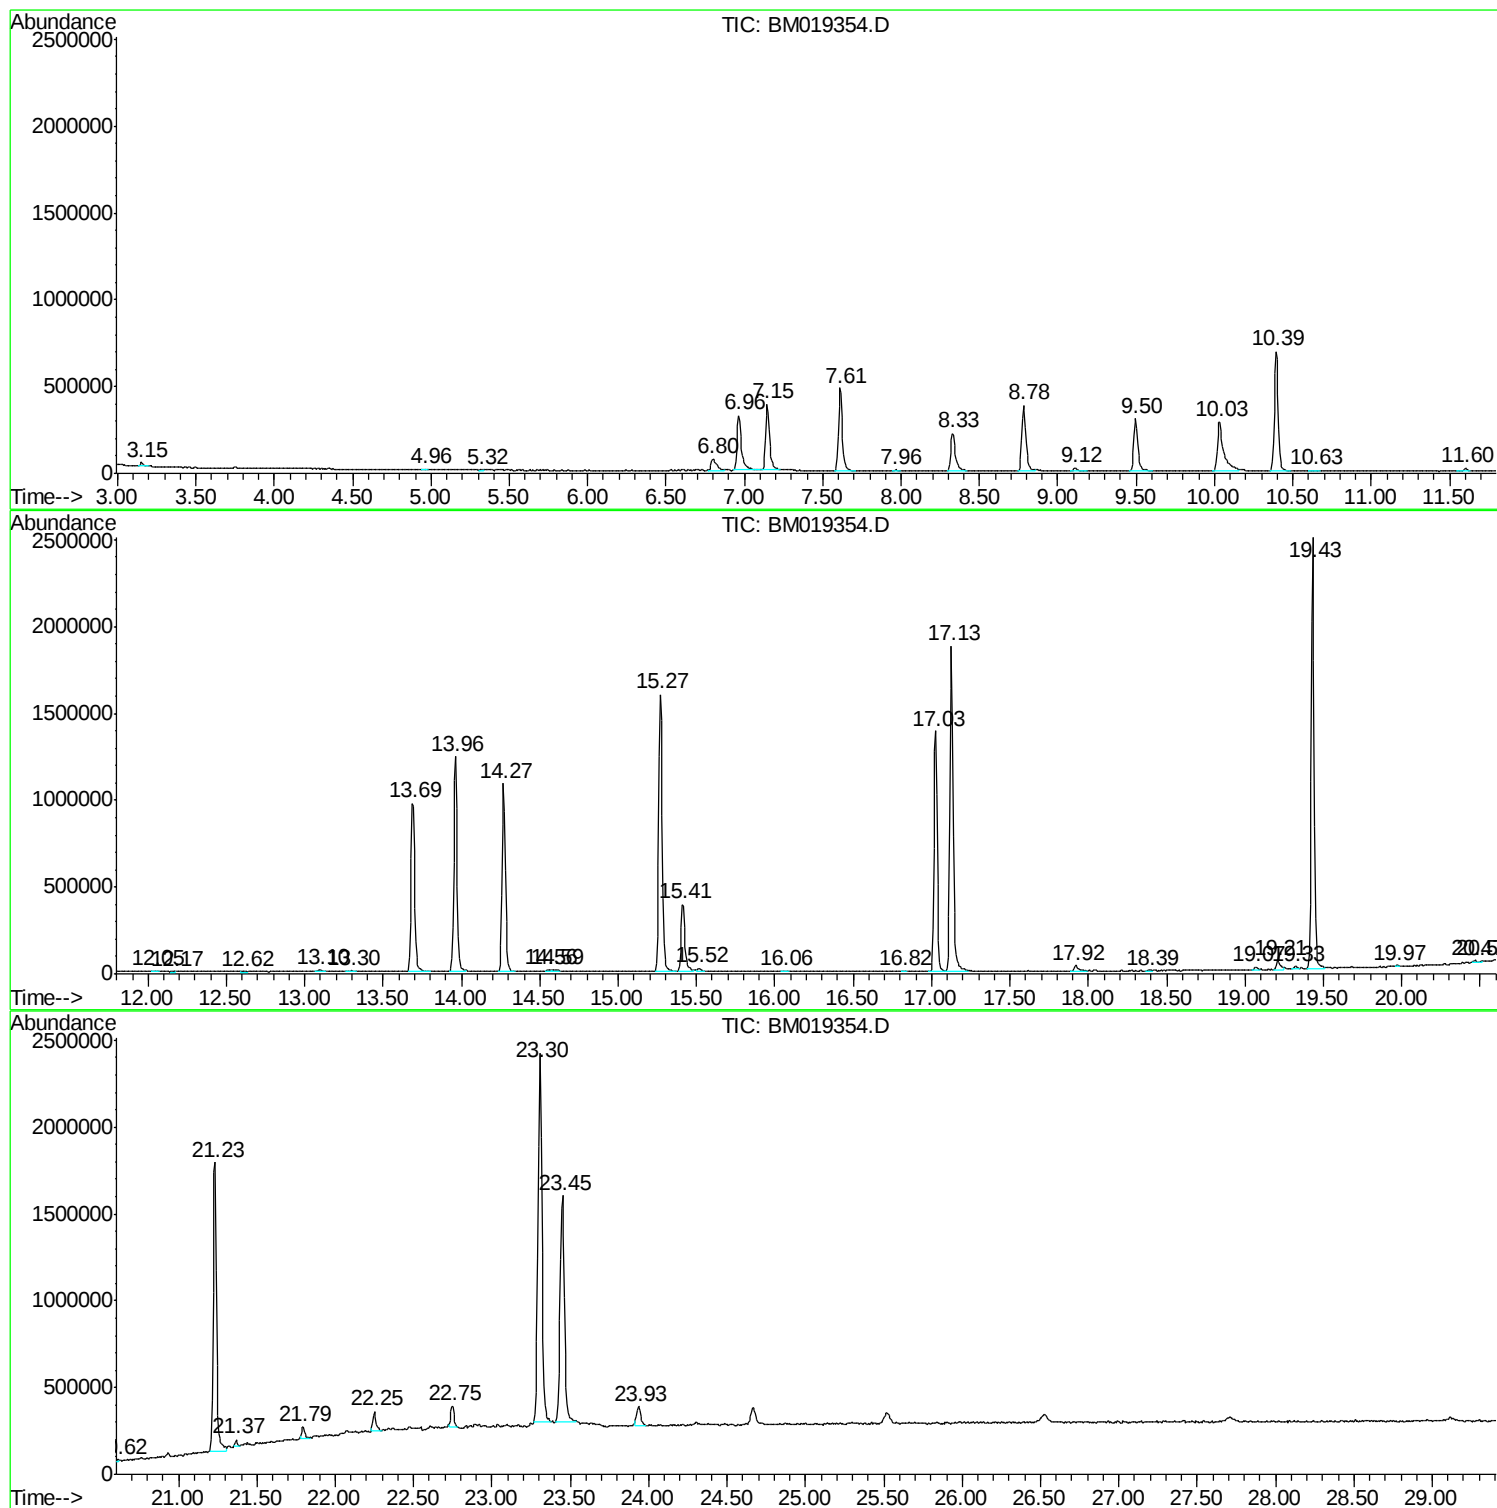

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
Data File : BM019354.D
Acq On : 23 Mar 2019 16:23
Operator : JU/SJ
Sample : K2025-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0982

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032319\
Data File : BM019354.D
Acq On : 23 Mar 2019 16:23
Operator : JU/SJ
Sample : K2025-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0982

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc