

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025707.D
 Acq On : 24 Mar 2020 00:19
 Operator : CG/JU
 Sample : L1890-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DB3

Quant Time: Mar 24 02:26:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 00:45:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	200003	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	805713	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	494005	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1060281	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1152215	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1303672	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	6884	1.44	ng/uL	0.00
5) Phenol-d5	6.76	99	115415	7.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	285964	31.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	338388	26.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	216427	16.69	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	213878	35.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	224635	35.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	399465	30.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	33771	2.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1389396	37.01	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1618961	35.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	46481	6.50	ng/ul	0.00
58) Fluorene-d10	15.21	176	1218072	36.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	190117	29.39	ng/ul	0.00
71) Anthracene-d10	17.06	188	1959775	39.57	ng/ul	0.00
79) Pyrene-d10	19.36	212	2140159	38.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2736123	40.99	ng/ul	0.00

Target Compounds


					Ovalue
33) 4-Chloro-3-methylphenol	11.63	107	26134	1.946 ng/ul	98
45) Dimethylphthalate	13.67	163	200996	5.143 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025707.D
Acq On : 24 Mar 2020 00:19
Operator : CG/JU
Sample : L1890-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DB3

Quant Time: Mar 24 02:26:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 00:45:06 2020
Response via : Initial Calibration




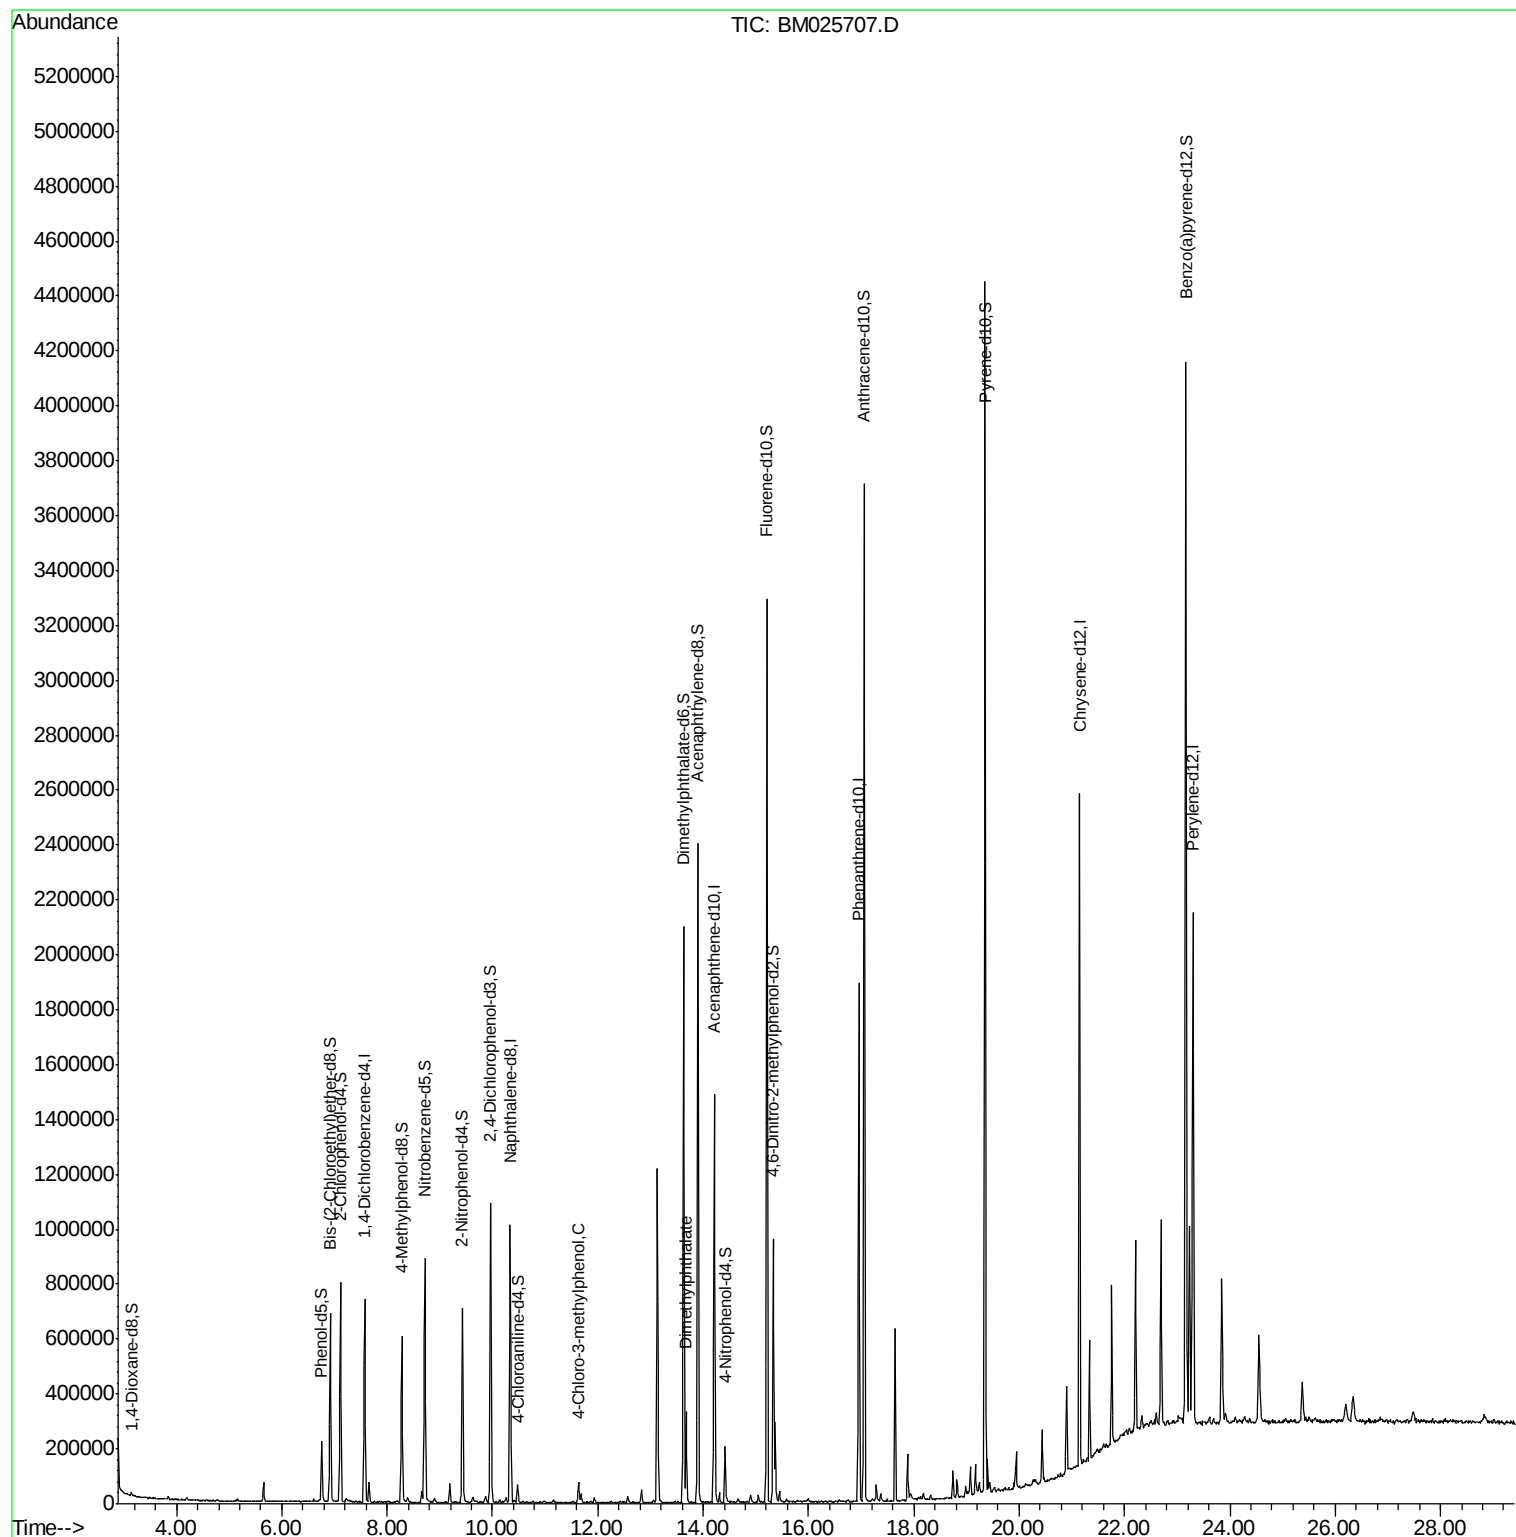


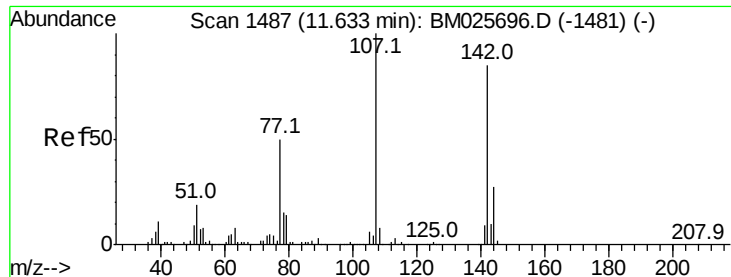

#33
 4-Chloro-3-methylphenol
 Concen: 1.946 ng/ul
 RT: 11.63 min Scan# 1487
 Delta R.T. -0.01 min
 Lab File: BM025707.D
 Acq: 24 Mar 2020 00:19

Instrument :
 BNA_M
 ClientSampleId :
 C0DB3

Tot Ion:107 Resp: 26134
 Ion Ratio Lower Upper
 107 100
 144 25.2 21.7 32.5
 142 79.6 65.0 97.6

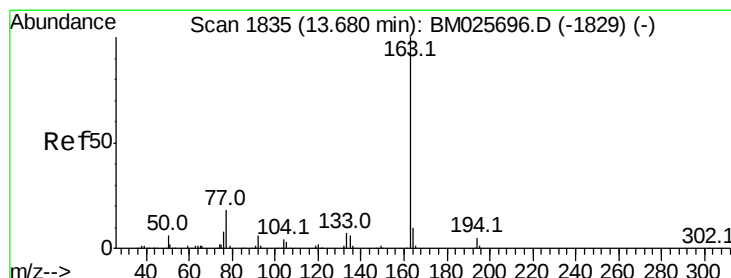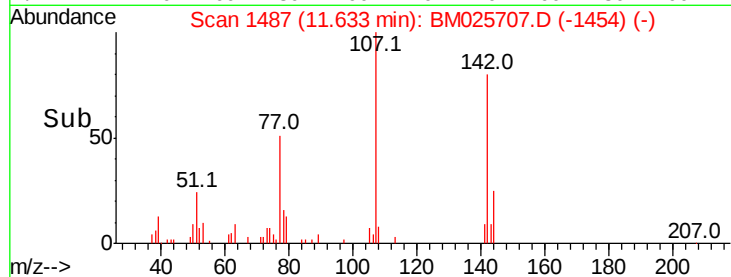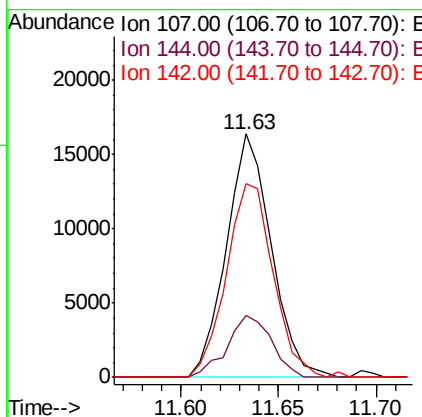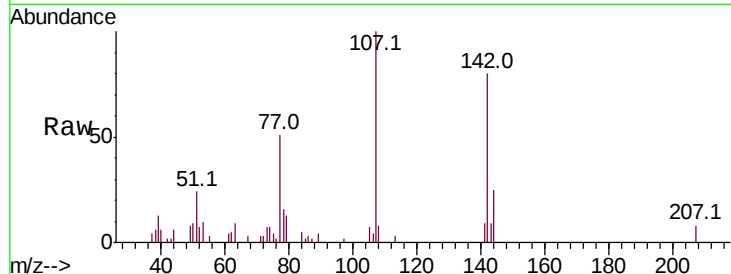

#45
 Dimethylphthalate
 Concen: 5.143 ng/ul
 RT: 13.67 min Scan# 1834
 Delta R.T. -0.01 min
 Lab File: BM025707.D
 Acq: 24 Mar 2020 00:19

Tgt Ion:163 Resp: 200996
 Ion Ratio Lower Upper
 163 100
 194 4.5 3.5 5.3
 164 9.9 8.2 12.4

