

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025714.D
 Acq On : 24 Mar 2020 05:06
 Operator : CG/JU
 Sample : L1890-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DH3

Quant Time: Mar 24 05:58:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 04:07:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	170725	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	690723	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	435282	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	969500	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1120369	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1279710	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	6850	1.68	ng/uL	0.00
5) Phenol-d5	6.76	99	111428	8.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	241823	31.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	299708	27.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	193504	17.48	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	175245	34.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	189112	34.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	348780	31.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	33930	2.62	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1286476	38.89	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1424213	35.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	53456	8.49	ng/ul	0.00
58) Fluorene-d10	15.21	176	1136644	39.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	197265	33.35	ng/ul	0.00
71) Anthracene-d10	17.06	188	1902218	42.01	ng/ul	0.00
79) Pyrene-d10	19.35	212	2157768	40.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2790164	42.59	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	193328	5.614	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025714.D
Acq On : 24 Mar 2020 05:06
Operator : CG/JU
Sample : L1890-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DH3

Quant Time: Mar 24 05:58:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 04:07:11 2020
Response via : Initial Calibration

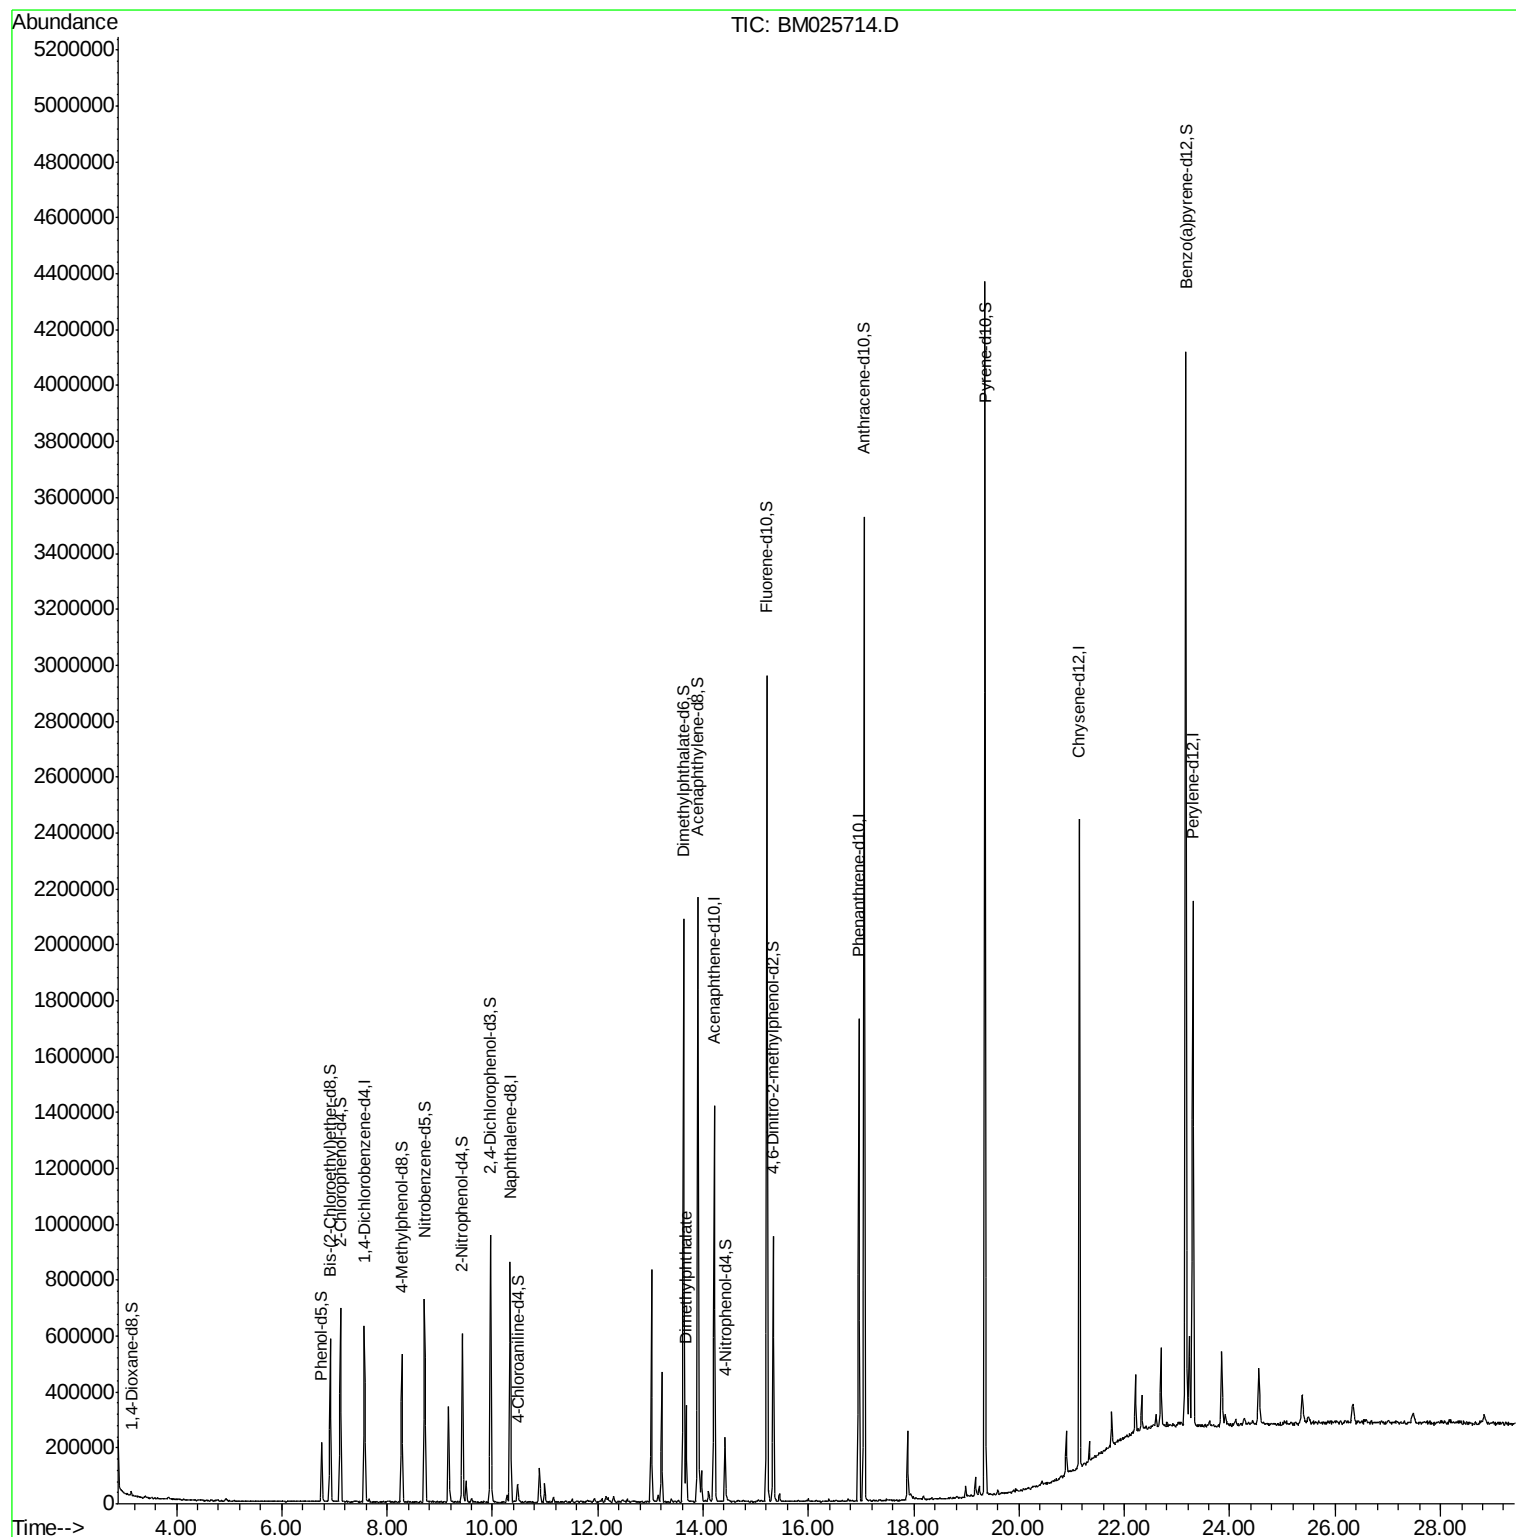

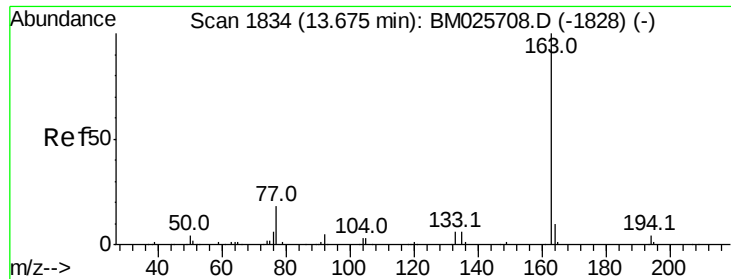

#45

Dimethylphthalate

Concen: 5.614 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM025714.D

Acq: 24 Mar 2020 05:06

Instrument :

BNA_M

ClientSampleId :

C0DH3



Tot Ion:163 Resp: 193328

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 9.7 8.2 12.4

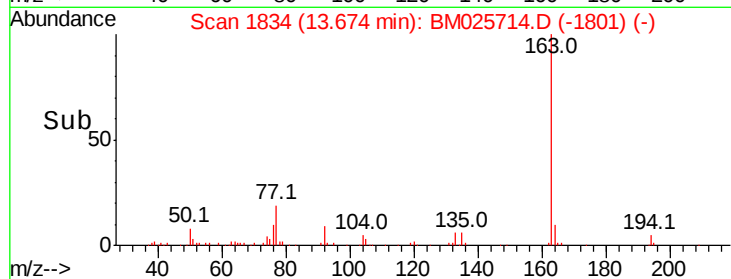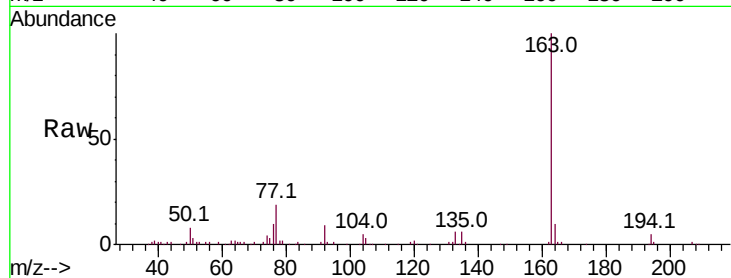

Abundance Ion 163.00 (162.70 to 163.70): E

200000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

