

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025726.D
 Acq On : 24 Mar 2020 12:54
 Operator : CG/JU
 Sample : L1940-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D90

Quant Time: Mar 24 13:40:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 00:45:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	170981	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	648329	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	410994	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	921463	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	1068466	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1200247	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	6210	1.52	ng/uL	0.00
5) Phenol-d5	6.76	99	85764	6.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	210539	27.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	254050	23.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	158485	14.29	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	149004	30.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	152201	29.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	278761	26.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	22597	1.86	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	963361	30.84	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1134896	30.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	33886	5.70	ng/ul	0.00
58) Fluorene-d10	15.21	176	883744	32.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	143988	25.61	ng/ul	0.00
71) Anthracene-d10	17.06	188	1524921	35.43	ng/ul	0.00
79) Pyrene-d10	19.35	212	1746433	34.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2207893	35.93	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	111320	3.424	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025726.D
Acq On : 24 Mar 2020 12:54
Operator : CG/JU
Sample : L1940-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D90

Quant Time: Mar 24 13:40:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 00:45:06 2020
Response via : Initial Calibration

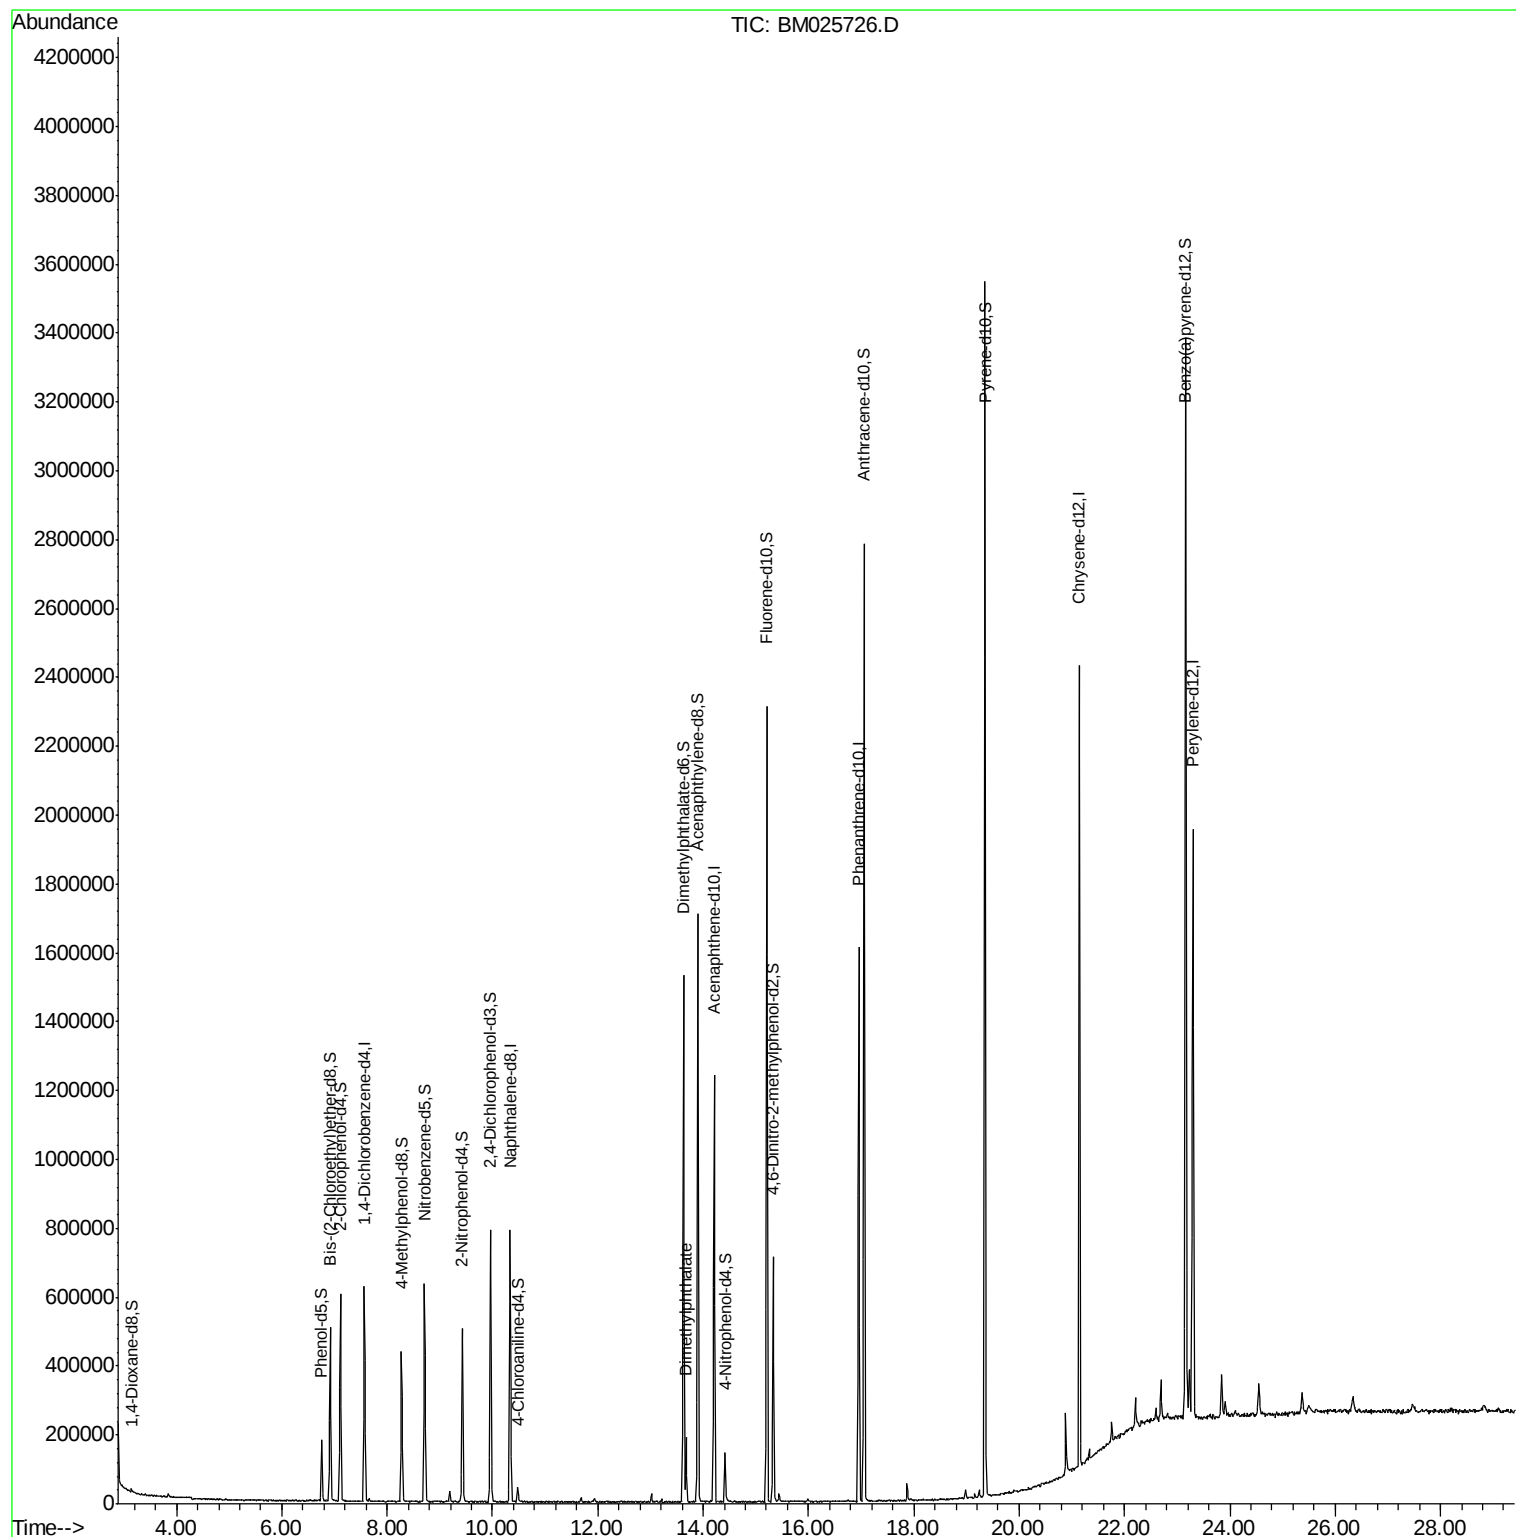

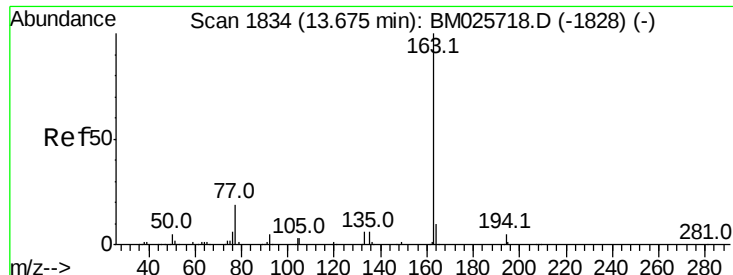

#45

Dimethylphthalate

Concen: 3.424 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM025726.D

Acq: 24 Mar 2020 12:54

Instrument :

BNA_M

ClientSampleId :

C0D90


Tot Ion:163 Resp: 111320

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 11.2 8.2 12.4

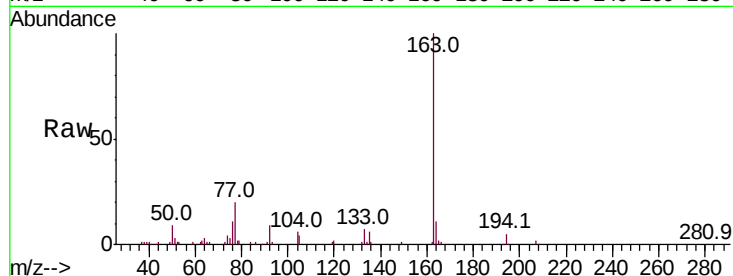

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

