

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025732.D
 Acq On : 24 Mar 2020 16:31
 Operator : CG/JU
 Sample : L1940-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D97

Quant Time: Mar 24 17:21:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 00:45:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	161920	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	641834	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	391181	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	873851	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	995385	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1129105	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	5103	1.32	ng/uL	0.00
5) Phenol-d5	6.76	99	71400	5.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	214550	29.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	245528	23.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	137860	13.13	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	152552	31.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	158446	31.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	282662	27.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	15801	1.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1004545	33.79	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1177984	33.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	25529	4.51	ng/ul	0.00
58) Fluorene-d10	15.21	176	902588	34.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	136263	25.56	ng/ul	0.00
71) Anthracene-d10	17.05	188	1463232	35.85	ng/ul	0.00
79) Pyrene-d10	19.35	212	1676810	35.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2143289	37.08	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	100733	3.255	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025732.D
Acq On : 24 Mar 2020 16:31
Operator : CG/JU
Sample : L1940-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D97

Quant Time: Mar 24 17:21:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 00:45:06 2020
Response via : Initial Calibration

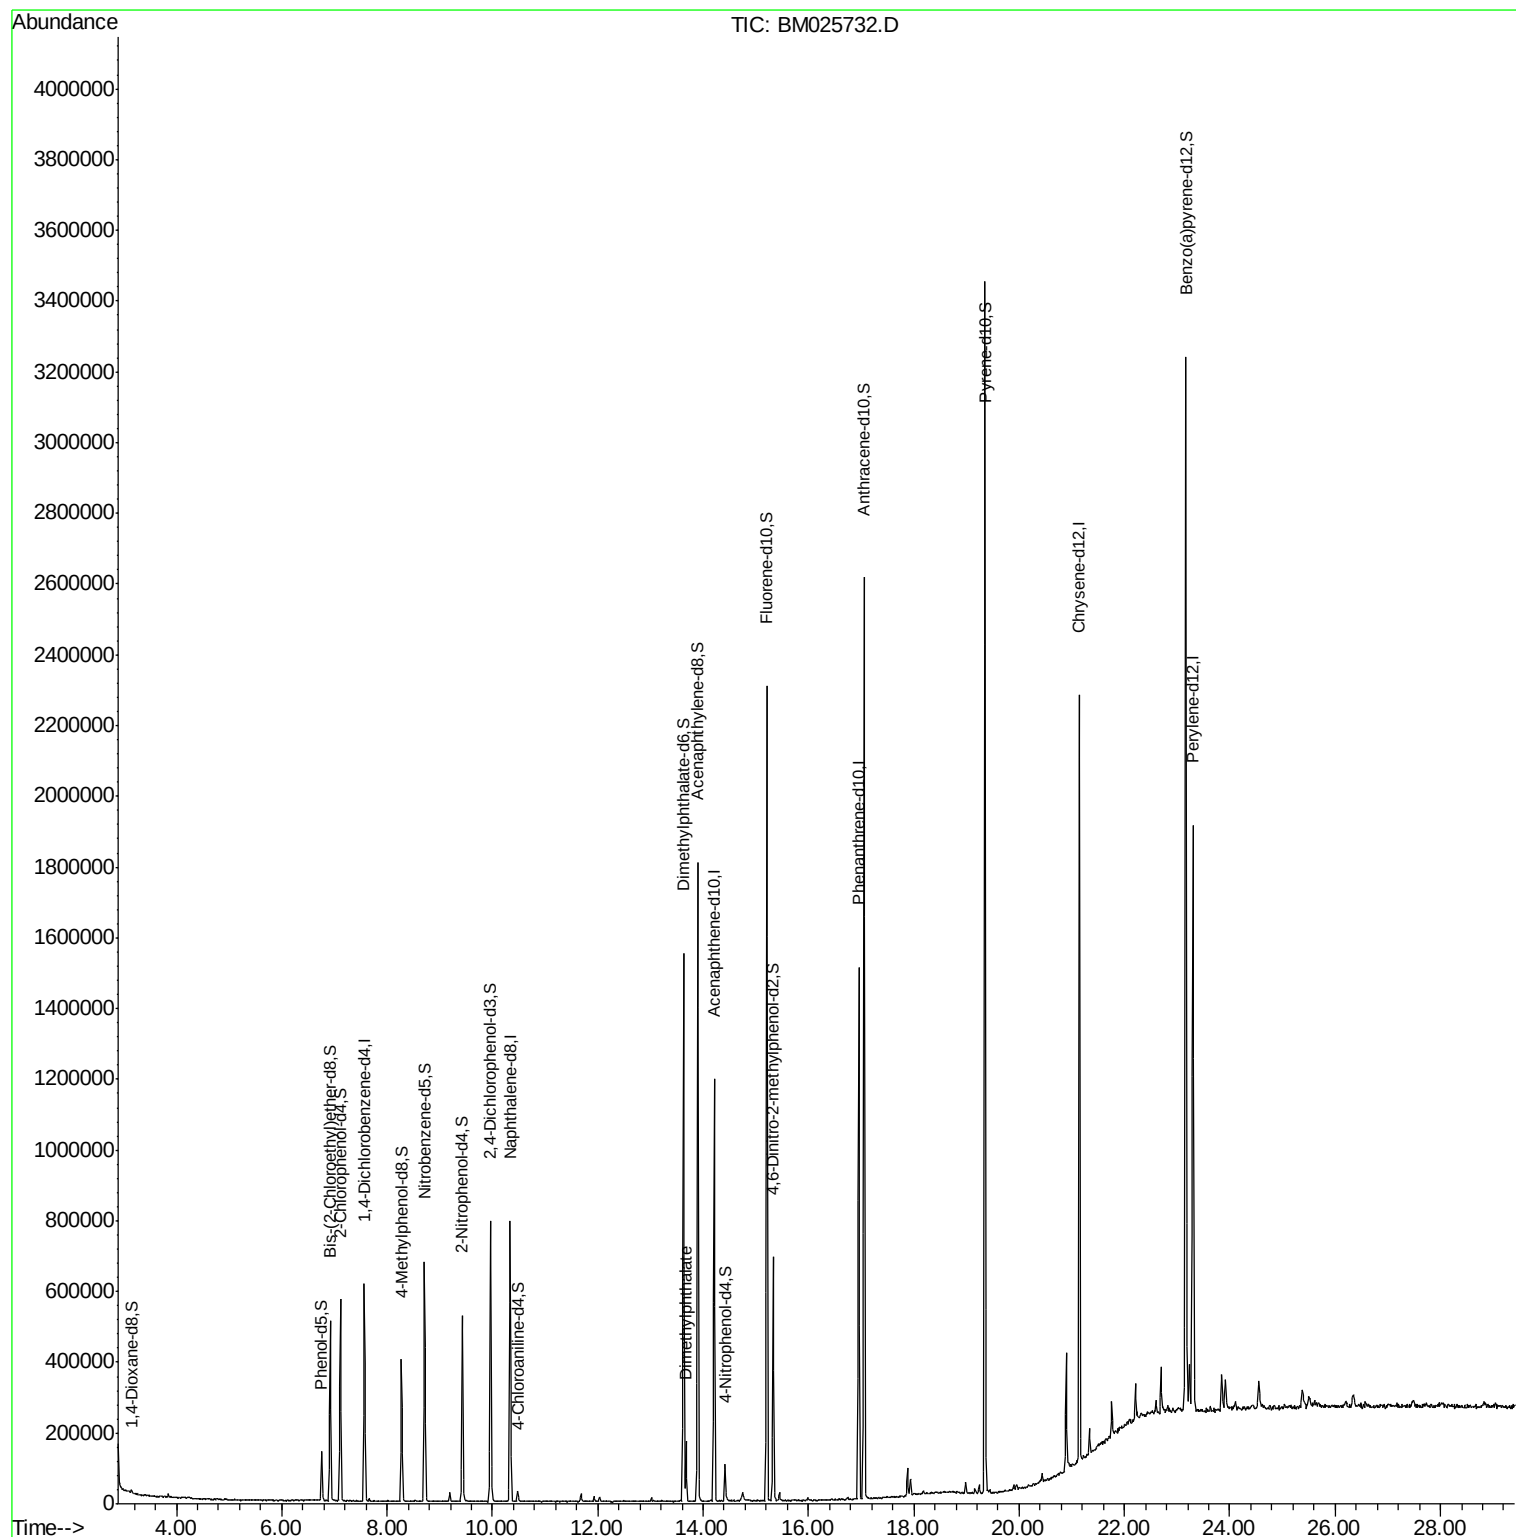

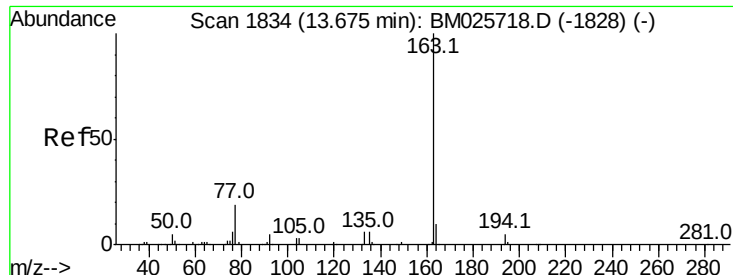

#45

Dimethylphthalate

Concen: 3.255 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM025732.D

Acq: 24 Mar 2020 16:31

Instrument :

BNA_M

ClientSampleId :

C0D97


Tot Ion:163 Resp: 100733

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 10.9 8.2 12.4

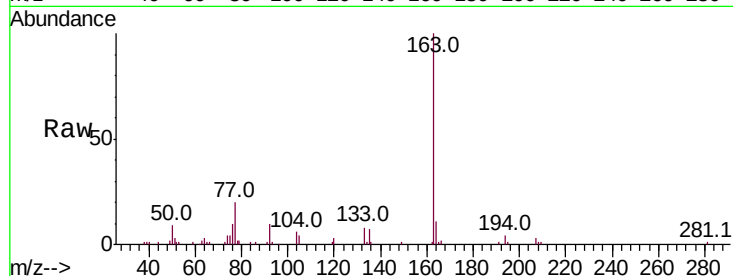

Abundance Ion 163.00 (162.70 to 163.70): E

100000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

