

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025740.D
 Acq On : 24 Mar 2020 21:56
 Operator : CG/JU
 Sample : L1940-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DB0

Quant Time: Mar 24 23:21:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 23:08:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	192363	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	782363	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.21	164	499757	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1102021	20.00	ng/ul	-0.01
78) Chrysene-d12	21.14	240	1213906	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1337044	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	6042	1.32	ng/uL	0.00
5) Phenol-d5	6.76	99	86485	5.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	250174	28.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	293815	23.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	177845	14.26	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	182596	31.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	192141	31.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	359598	28.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	22612	1.54	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1281030	33.73	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1507843	33.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	32697	4.52	ng/ul	0.00
58) Fluorene-d10	15.20	176	1143519	34.30	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.33	200	180493	26.84	ng/ul	-0.01
71) Anthracene-d10	17.05	188	1840417	35.75	ng/ul	0.00
79) Pyrene-d10	19.35	212	2033601	34.88	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2492616	36.41	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	102283	2.587	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025740.D
Acq On : 24 Mar 2020 21:56
Operator : CG/JU
Sample : L1940-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DB0

Quant Time: Mar 24 23:21:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 23:08:23 2020
Response via : Initial Calibration

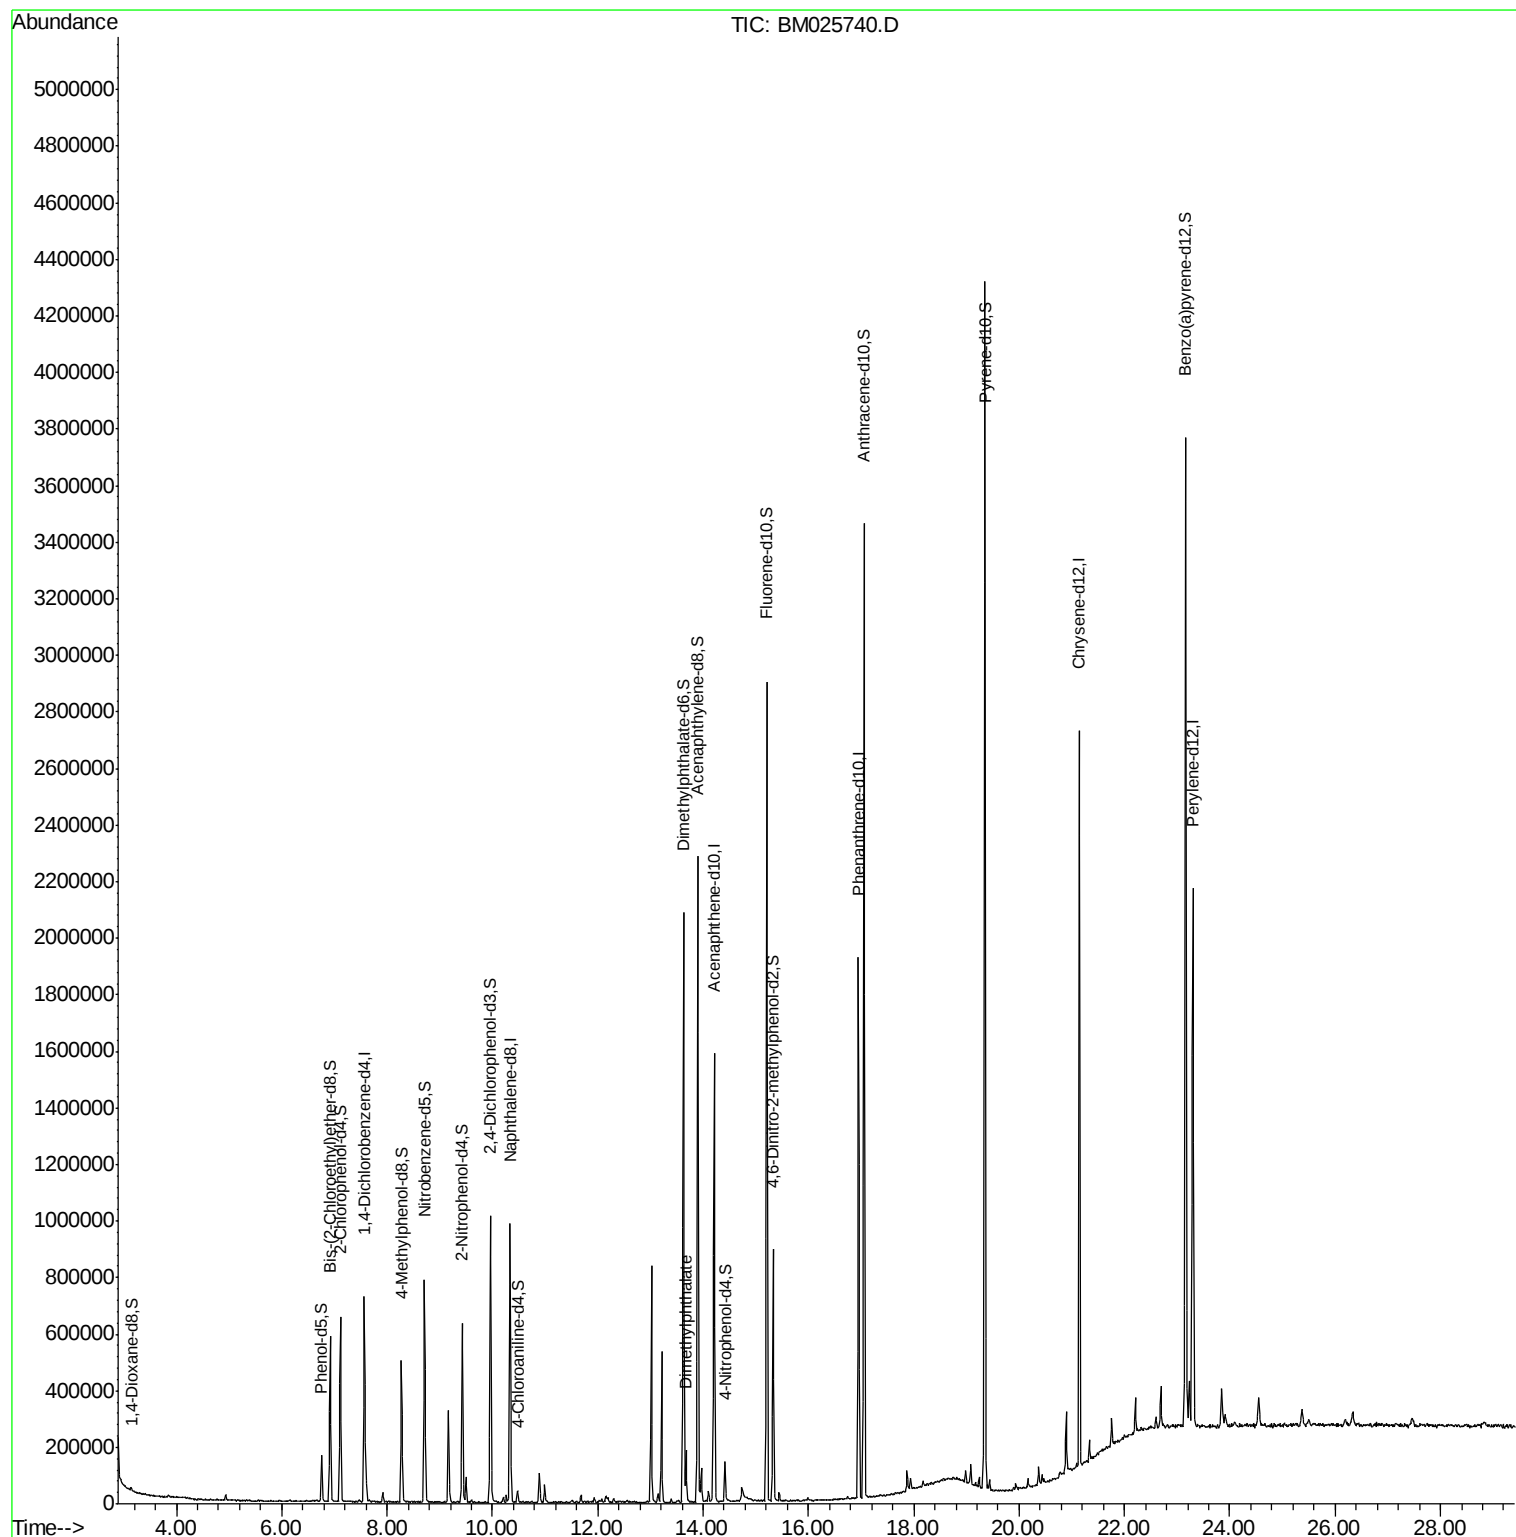

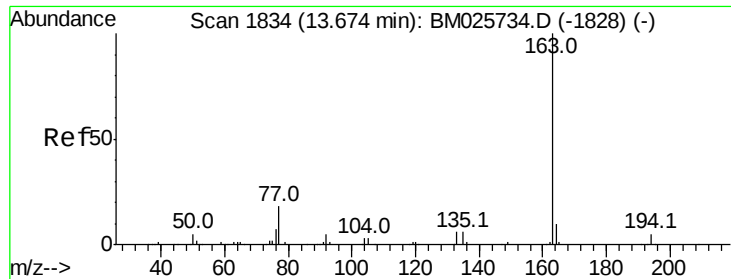

#45

Dimethylphthalate

Concen: 2.587 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM025740.D

Acq: 24 Mar 2020 21:56

Instrument :

BNA_M

ClientSampleId :

C0DB0



Tot Ion:163 Resp: 102283

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.2 8.2 12.4

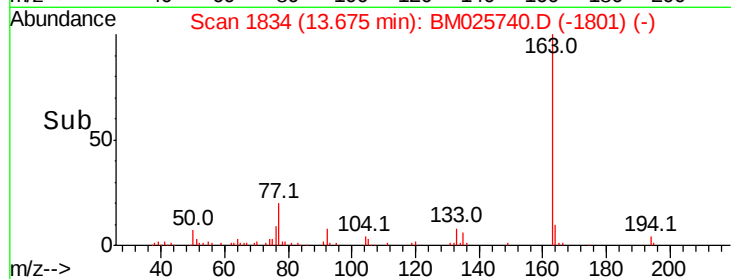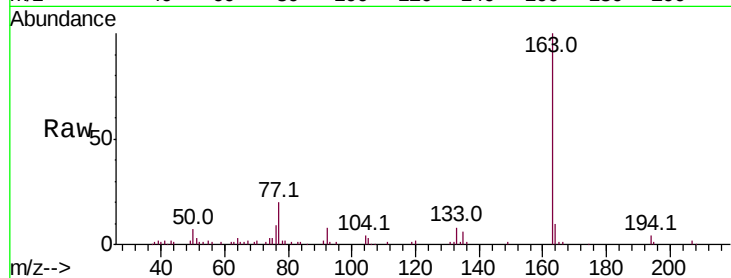

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

