

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025745.D
 Acq On : 25 Mar 2020 00:56
 Operator : CG/JU
 Sample : L1940-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DA6

Quant Time: Mar 25 02:10:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 23:08:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	209567	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	865972	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.21	164	544559	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1192340	20.00	ng/ul	-0.01
78) Chrysene-d12	21.14	240	1274823	20.00	ng/ul	-0.01
86) Perylene-d12	23.29	264	1433863	20.00	ng/ul	-0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	6378	1.28	ng/uL	0.00
5) Phenol-d5	6.75	99	98290	5.94	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.92	67	275979	29.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	325913	24.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	202473	14.90	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	205501	31.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	218423	31.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	408358	29.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	19126	1.18	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1383545	33.43	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1643582	33.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	37997	4.82	ng/ul	0.00
58) Fluorene-d10	15.20	176	1244091	34.24	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.33	200	192570	26.47	ng/ul	-0.01
71) Anthracene-d10	17.05	188	1912106	34.33	ng/ul	0.00
79) Pyrene-d10	19.35	212	2133670	34.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2634109	35.88	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	62299	1.446	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025745.D
Acq On : 25 Mar 2020 00:56
Operator : CG/JU
Sample : L1940-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA6

Quant Time: Mar 25 02:10:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 23:08:23 2020
Response via : Initial Calibration

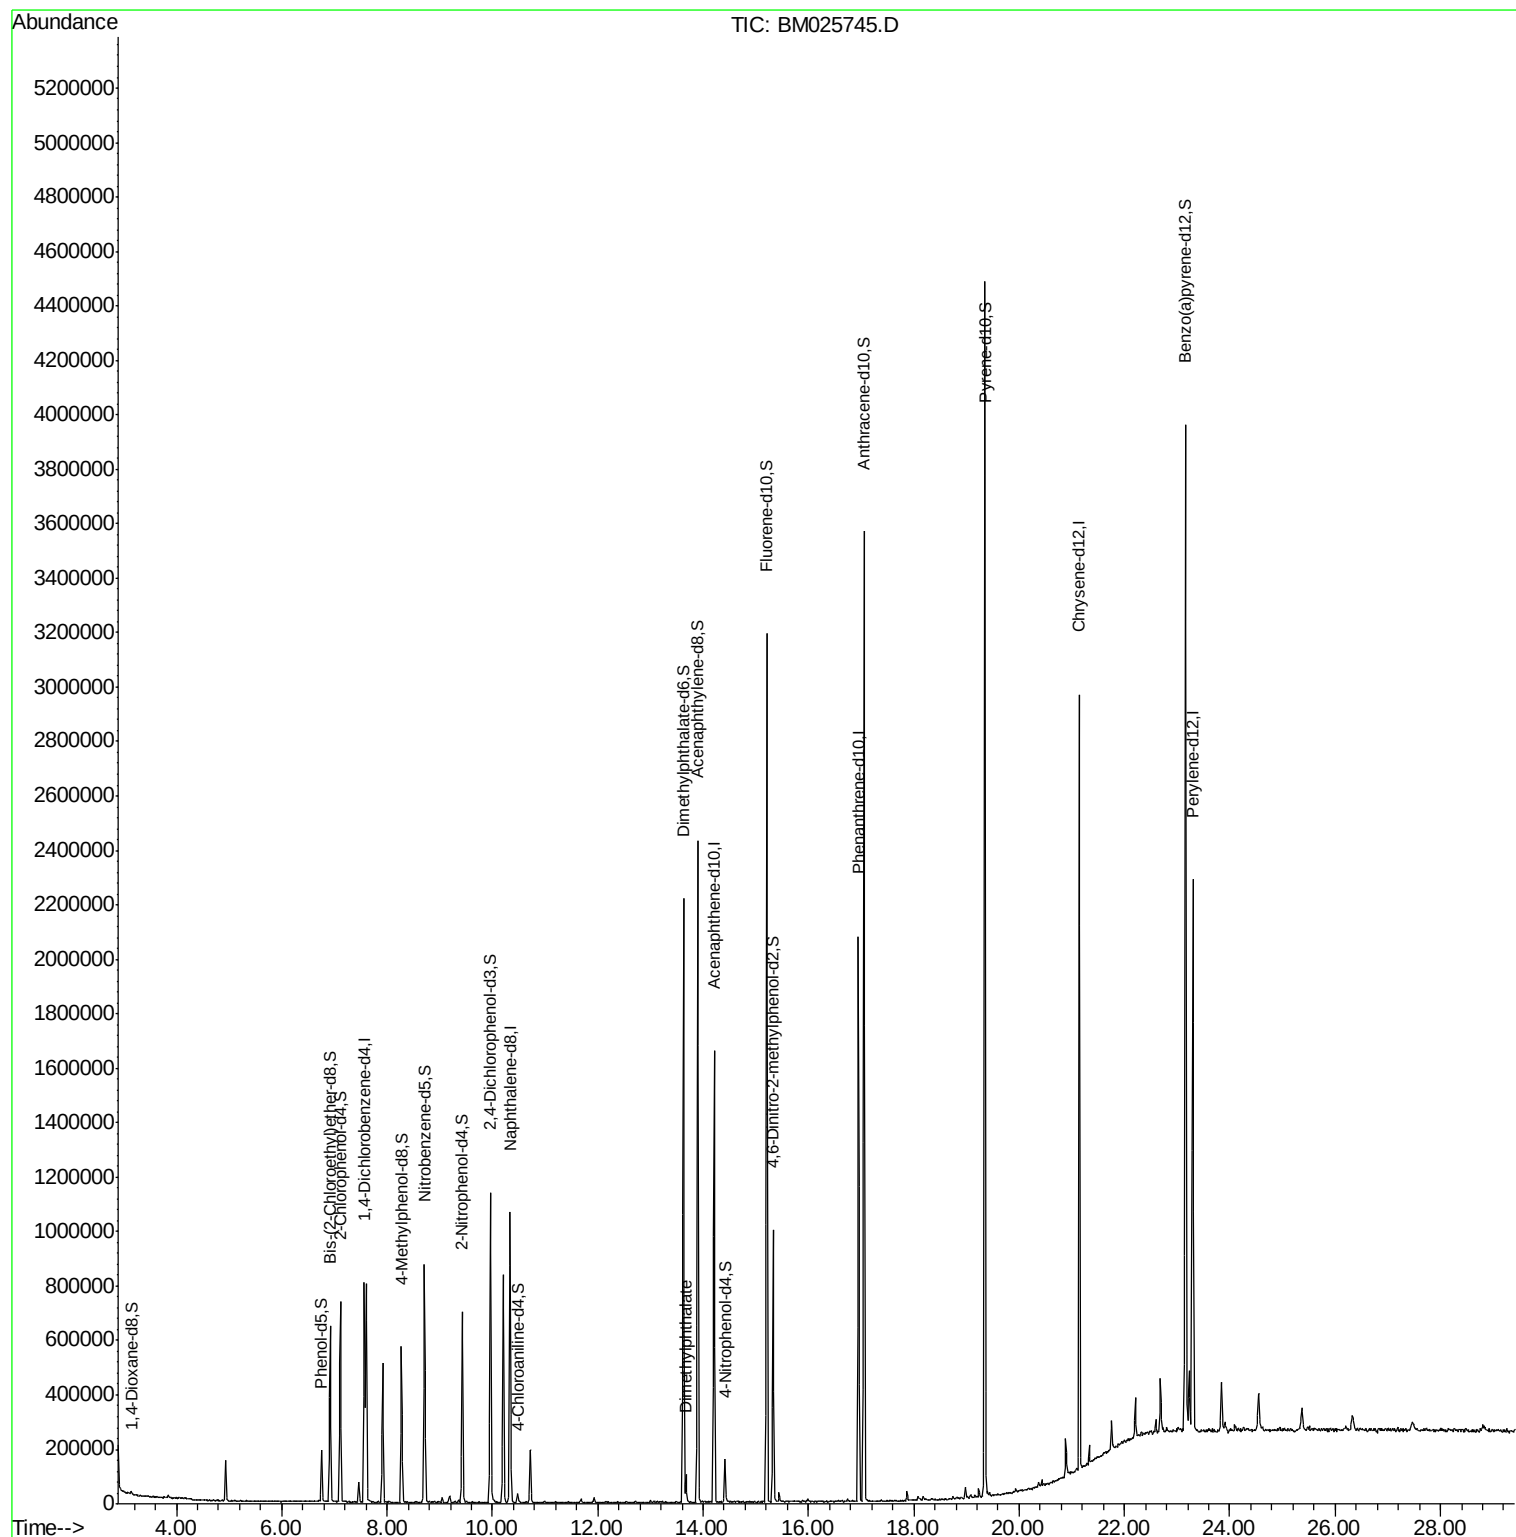

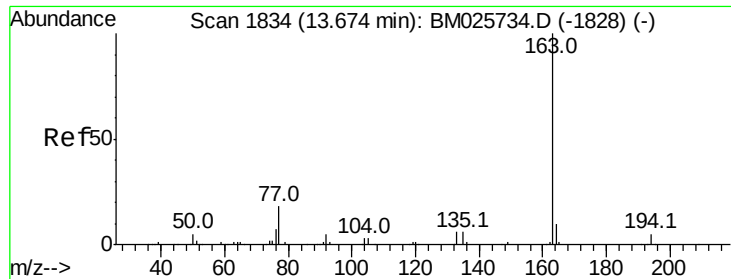

#45

Dimethylphthalate

Concen: 1.446 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM025745.D

Acq: 25 Mar 2020 00:56

Instrument :

BNA_M

ClientSampleId :

C0DA6


Tot Ion:163 Resp: 62299

Ion Ratio Lower Upper

163 100

194 5.0 3.5 5.3

164 10.2 8.2 12.4

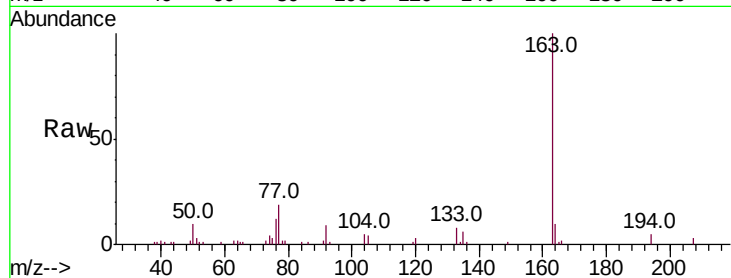

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

