

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025751.D
 Acq On : 25 Mar 2020 05:08
 Operator : CG/JU
 Sample : L1938-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB727

Quant Time: Mar 25 06:13:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 23:08:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	207848	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	868440	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.21	164	555974	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1191924	20.00	ng/ul	-0.01
78) Chrysene-d12	21.14	240	1227777	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1383860	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	21470	4.33	ng/uL	0.00
5) Phenol-d5	6.75	99	423958	25.84	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.91	67	246186	26.29	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	361708	27.17	ng/ul	-0.01
13) 4-Methylphenol-d8	8.27	113	355077	26.34	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	181053	28.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	193461	28.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	370021	26.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	502303	30.83	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1186131	28.07	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1422510	28.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	199998	24.86	ng/ul	0.00
58) Fluorene-d10	15.20	176	1048173	28.26	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.33	200	157295	21.63	ng/ul	-0.01
71) Anthracene-d10	17.05	188	1611285	28.94	ng/ul	0.00
79) Pyrene-d10	19.35	212	1844337	31.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2252686	31.79	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	165653	3.766	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025751.D
Acq On : 25 Mar 2020 05:08
Operator : CG/JU
Sample : L1938-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB727

Quant Time: Mar 25 06:13:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 23:08:23 2020
Response via : Initial Calibration

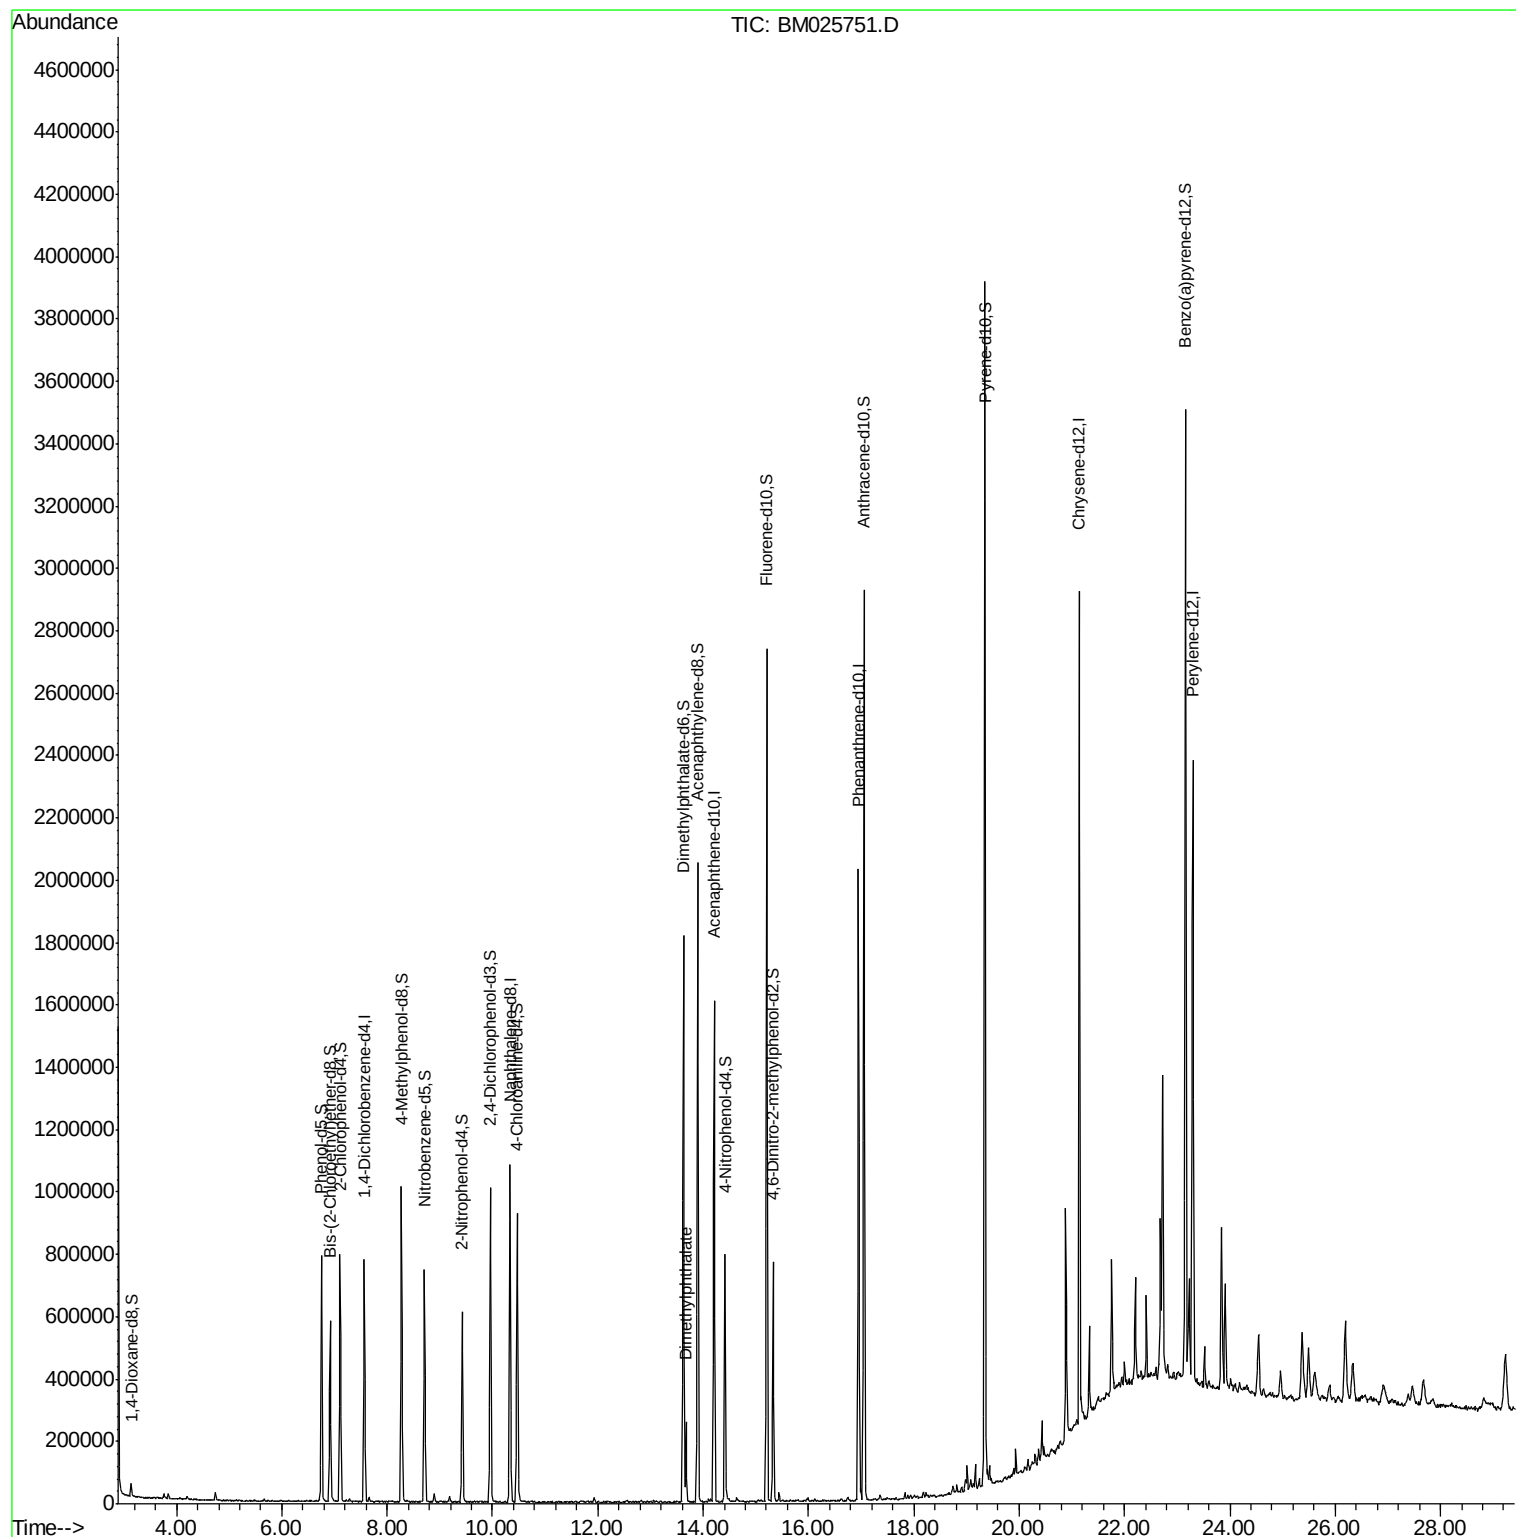

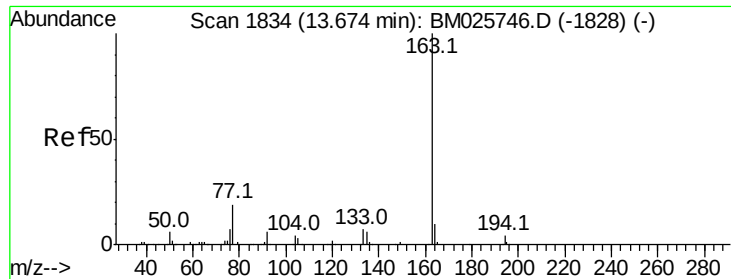

#45

Dimethylphthalate

Concen: 3.766 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM025751.D

Acq: 25 Mar 2020 05:08

Instrument :

BNA_M

ClientSampleId :

CB727



Tot Ion:163 Resp: 165653

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 9.9 8.2 12.4

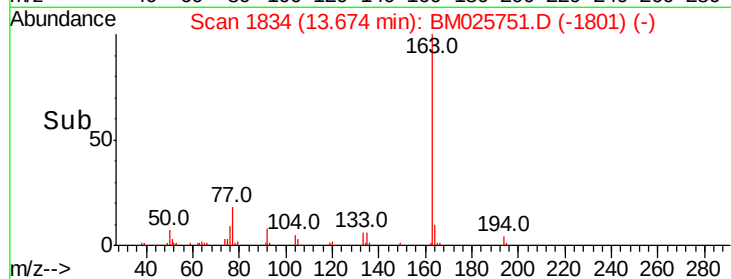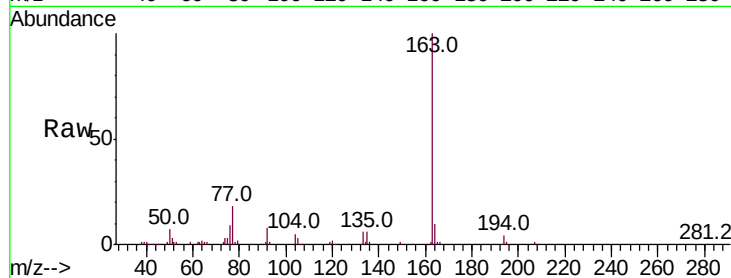

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

