

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025767.D
 Acq On : 25 Mar 2020 14:44
 Operator : CG/JU
 Sample : L1938-12
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB779

Quant Time: Mar 25 16:52:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 25 07:24:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	155667	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	656753	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.20	164	421069	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.95	188	905027	20.00	ng/ul	-0.01
78) Chrysene-d12	21.14	240	941179	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1059727	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	19675	5.30	ng/uL	0.00
5) Phenol-d5	6.75	99	352212	28.67	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.91	67	208054	29.67	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	300053	30.09	ng/ul	-0.01
13) 4-Methylphenol-d8	8.27	113	294488	29.17	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	150241	30.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	161292	31.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	304069	28.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	411553	33.40	ng/ul	-0.01
44) Dimethylphthalate-d6	13.63	166	990487	30.95	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1188863	31.01	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.41	143	164997	27.08	ng/ul	-0.01
58) Fluorene-d10	15.20	176	866679	30.85	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.33	200	134225	24.31	ng/ul	-0.01
71) Anthracene-d10	17.05	188	1348061	31.89	ng/ul	0.00
79) Pyrene-d10	19.35	212	1564669	34.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	1891044	34.85	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	135890	4.079	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025767.D
Acq On : 25 Mar 2020 14:44
Operator : CG/JU
Sample : L1938-12
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB779

Quant Time: Mar 25 16:52:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 25 07:24:39 2020
Response via : Initial Calibration

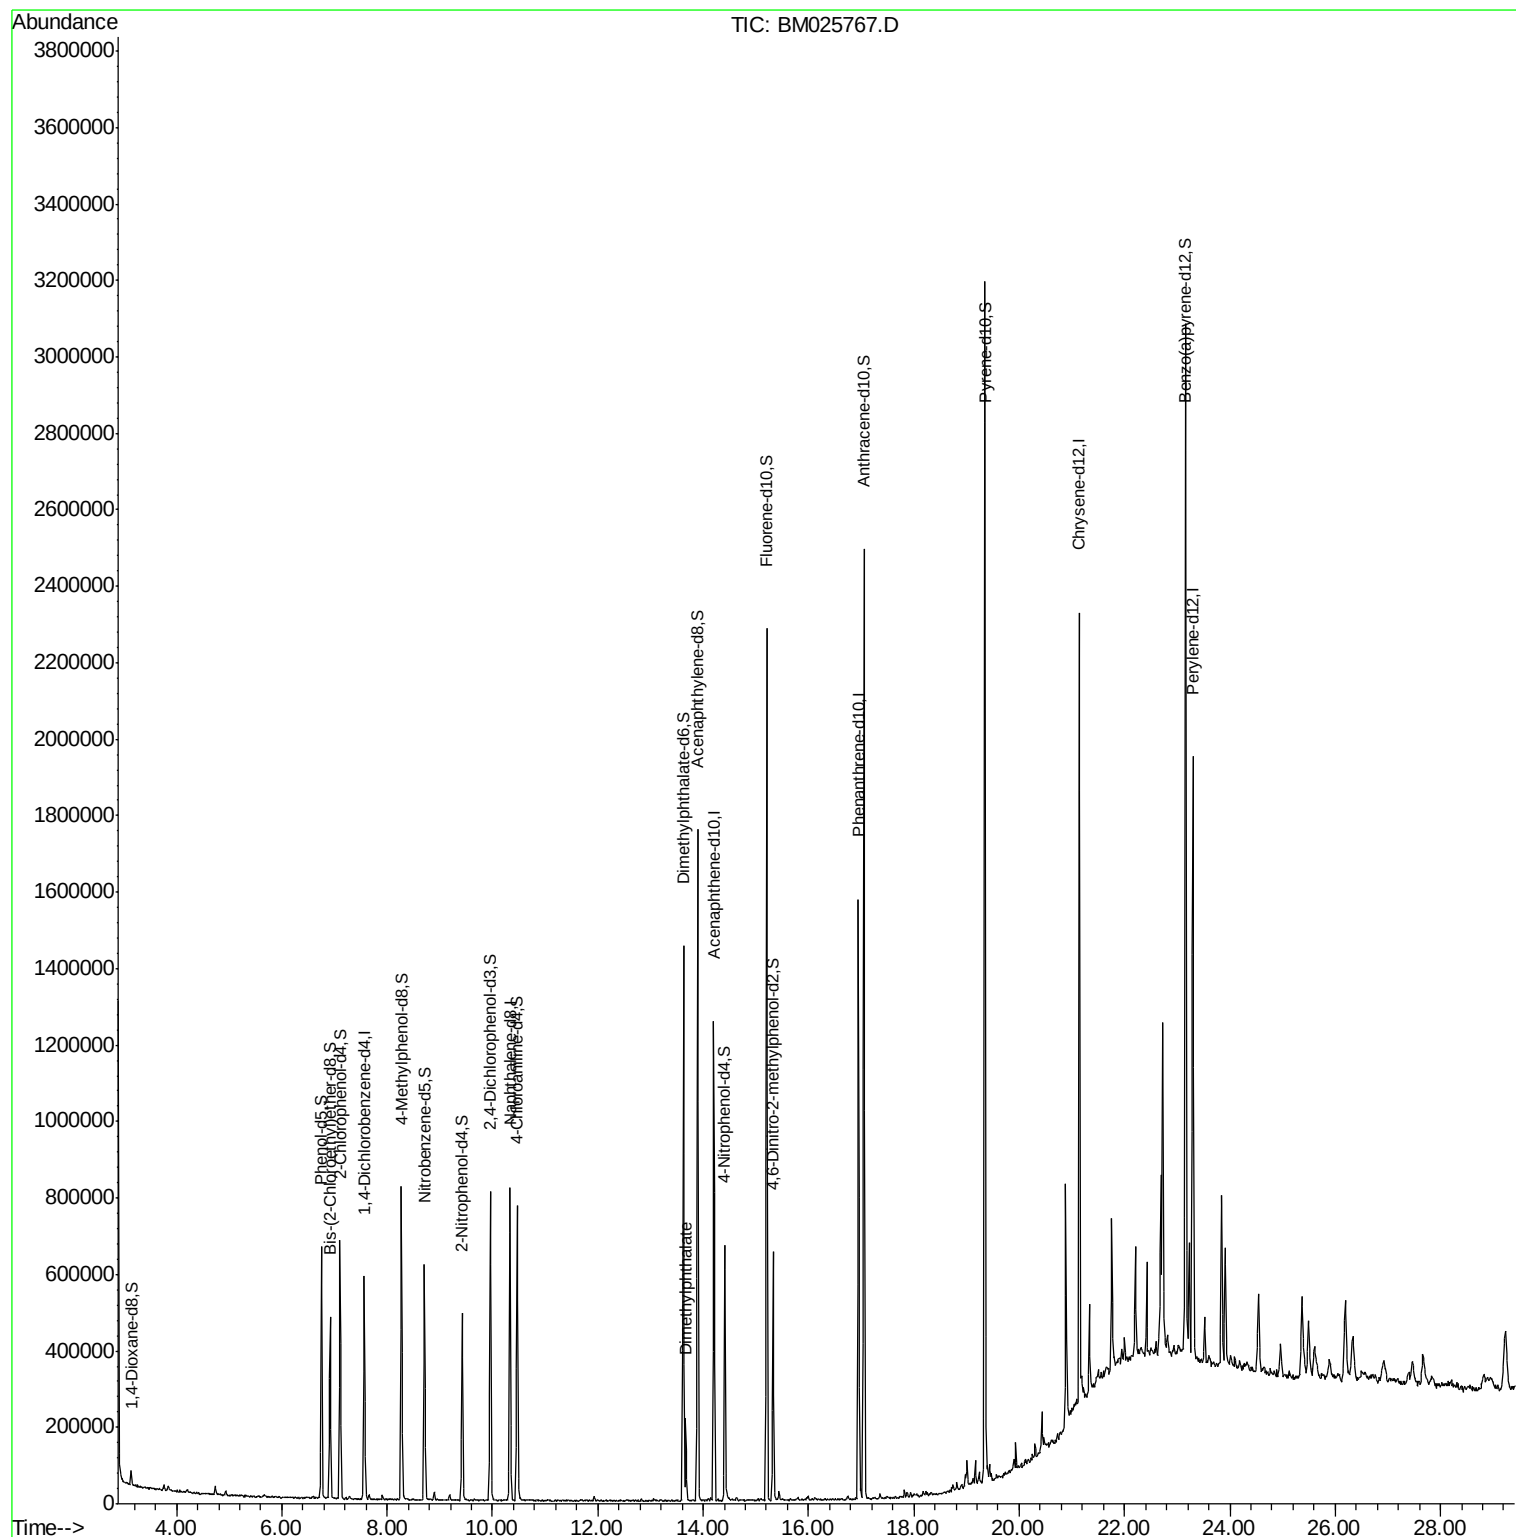

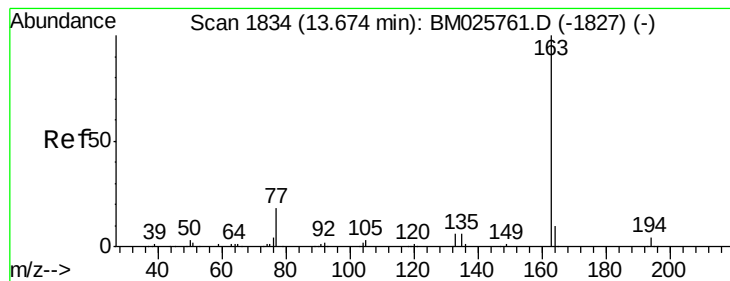

#45

Dimethylphthalate

Concen: 4.079 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BM025767.D

Acq: 25 Mar 2020 14:44

Instrument :

BNA_M

ClientSampleId :

CB779


Tot Ion:163 Resp: 135890

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.5 8.2 12.4

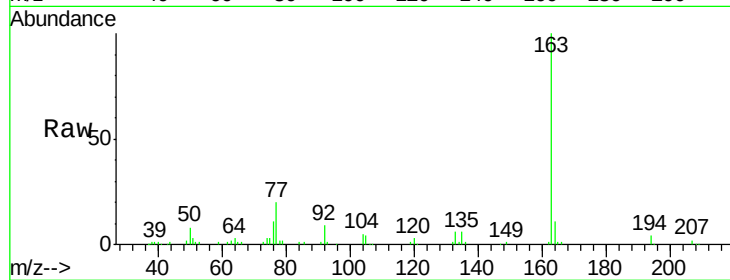

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

