

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025776.D
 Acq On : 25 Mar 2020 20:07
 Operator : CG/JU
 Sample : L1941-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DA3

Quant Time: Mar 26 00:50:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 00:45:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	187059	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	760787	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.20	164	473730	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.95	188	1023718	20.00	ng/ul	-0.01
78) Chrysene-d12	21.14	240	1083060	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1217214	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	5736	1.29	ng/uL	0.00
5) Phenol-d5	6.75	99	87248	5.91	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.91	67	237359	28.17	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	281011	23.45	ng/ul	-0.01
13) 4-Methylphenol-d8	8.27	113	170532	14.06	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	178769	31.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	192077	31.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	326866	26.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	19480	1.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1119134	31.08	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1358630	31.50	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.42	143	31073	4.53	ng/ul	0.00
58) Fluorene-d10	15.20	176	991052	31.36	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.33	200	155550	24.90	ng/ul	-0.01
71) Anthracene-d10	17.05	188	1612397	33.72	ng/ul	0.00
79) Pyrene-d10	19.35	212	1745987	33.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2136950	34.29	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	76039	2.029	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025776.D
Acq On : 25 Mar 2020 20:07
Operator : CG/JU
Sample : L1941-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA3

Quant Time: Mar 26 00:50:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 00:45:06 2020
Response via : Initial Calibration

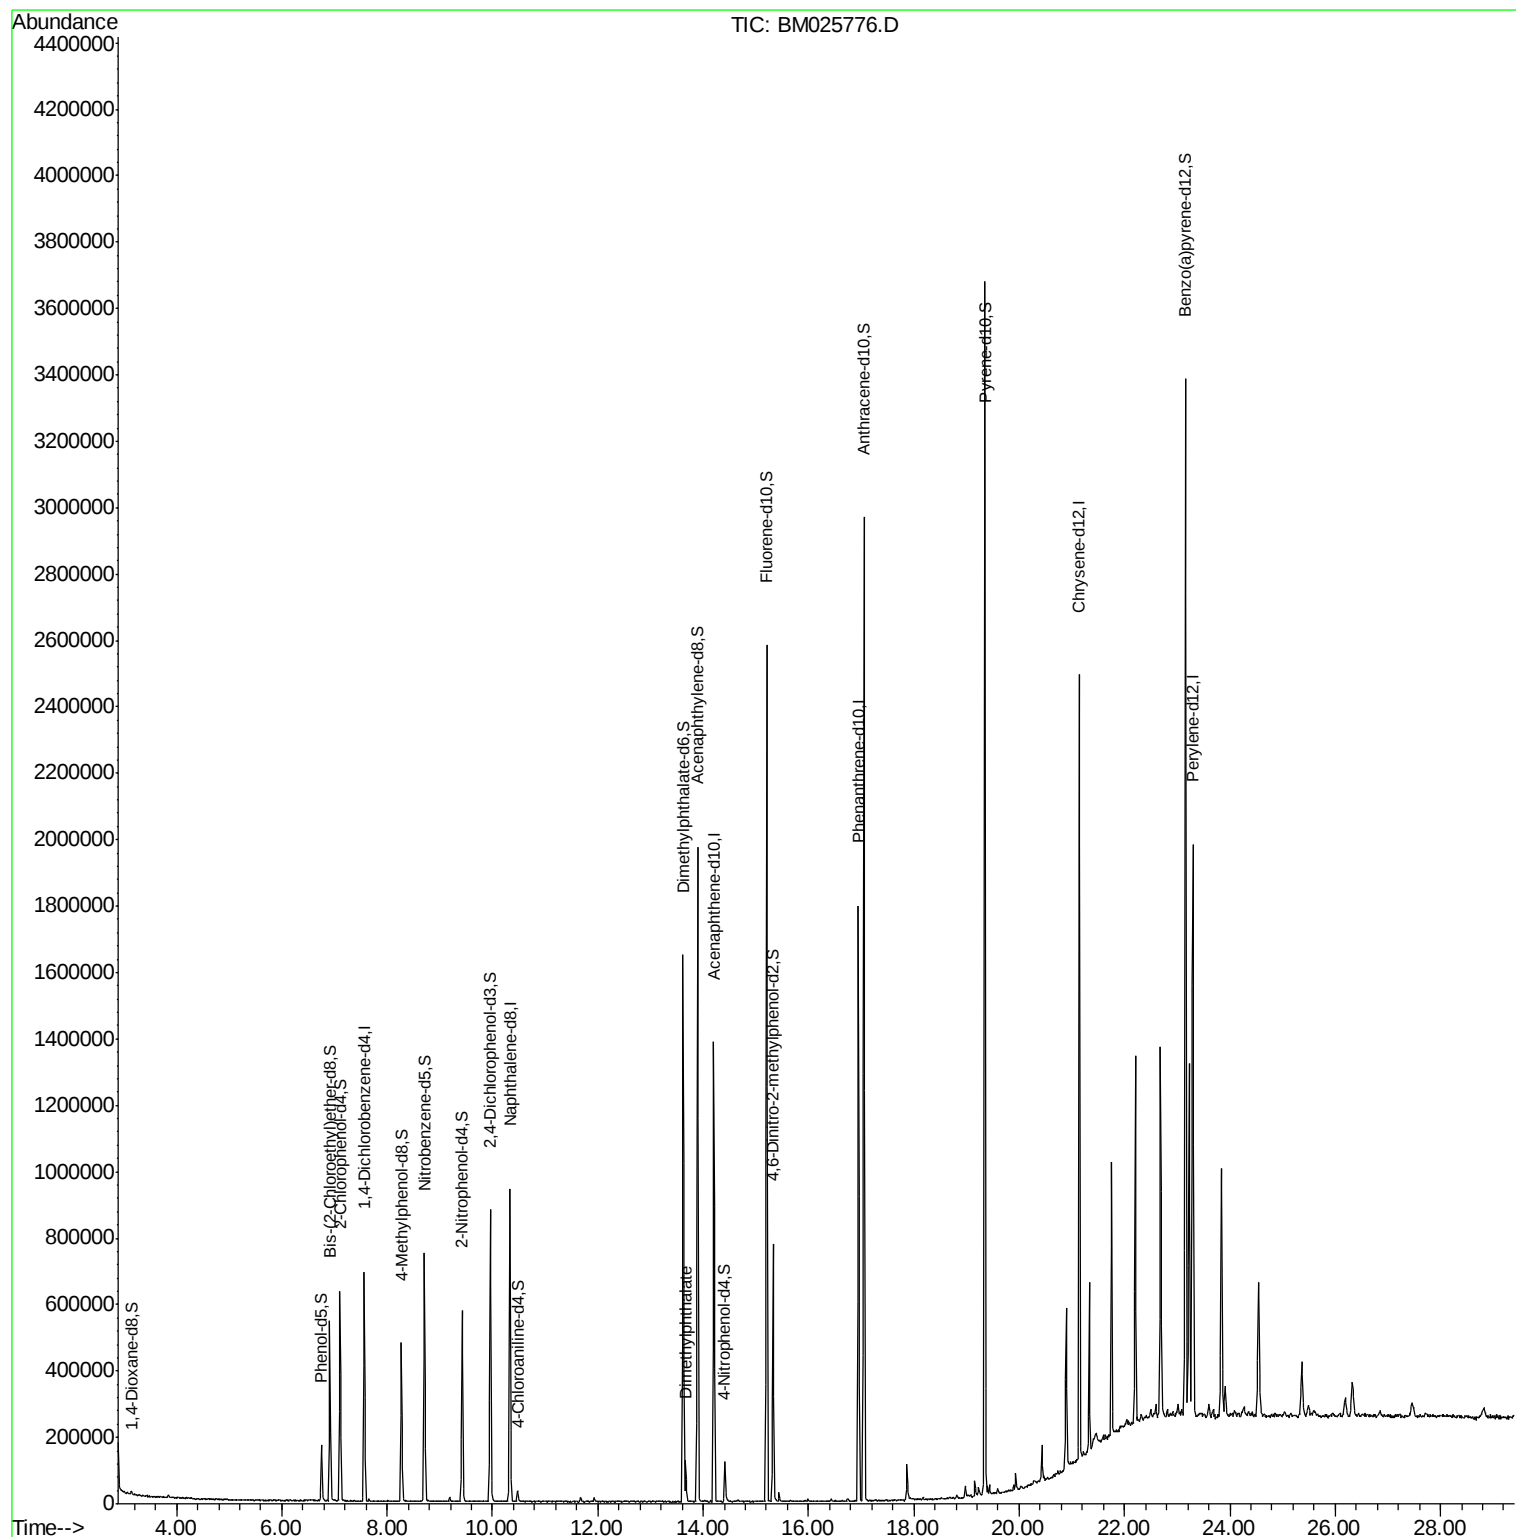

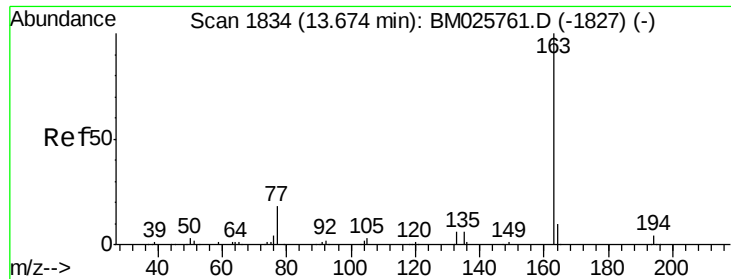

#45

Dimethylphthalate

Concen: 2.029 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BM025776.D

Acq: 25 Mar 2020 20:07

Instrument :

BNA_M

ClientSampleId :

C0DA3


Tot Ion:163 Resp: 76039

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.6 8.2 12.4

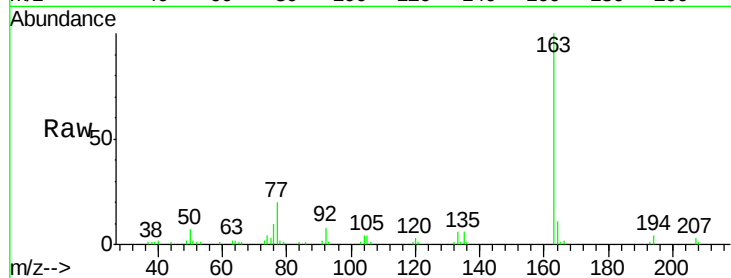

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

