

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025778.D
 Acq On : 25 Mar 2020 21:19
 Operator : CG/JU
 Sample : L1941-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DA4

Quant Time: Mar 26 01:00:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 24 00:45:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	205288	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	846449	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.20	164	533042	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.95	188	1146086	20.00	ng/ul	-0.01
78) Chrysene-d12	21.14	240	1248705	20.00	ng/ul	-0.01
86) Perylene-d12	23.30	264	1399007	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	6341	1.30	ng/uL	0.00
5) Phenol-d5	6.75	99	93790	5.79	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.91	67	266218	28.79	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	306092	23.28	ng/ul	-0.01
13) 4-Methylphenol-d8	8.27	113	189425	14.23	ng/ul	-0.01
19) Nitrobenzene-d5	8.71	128	201018	31.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	215112	32.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	371715	27.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	25139	1.58	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1325242	32.71	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1554891	32.04	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.41	143	36357	4.71	ng/ul	-0.01
58) Fluorene-d10	15.20	176	1169373	32.88	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.33	200	191153	27.34	ng/ul	-0.01
71) Anthracene-d10	17.05	188	1913312	35.74	ng/ul	0.00
79) Pyrene-d10	19.35	212	2072972	34.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2597493	36.26	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	70135	1.663	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025778.D
Acq On : 25 Mar 2020 21:19
Operator : CG/JU
Sample : L1941-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA4

Quant Time: Mar 26 01:00:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 24 00:45:06 2020
Response via : Initial Calibration

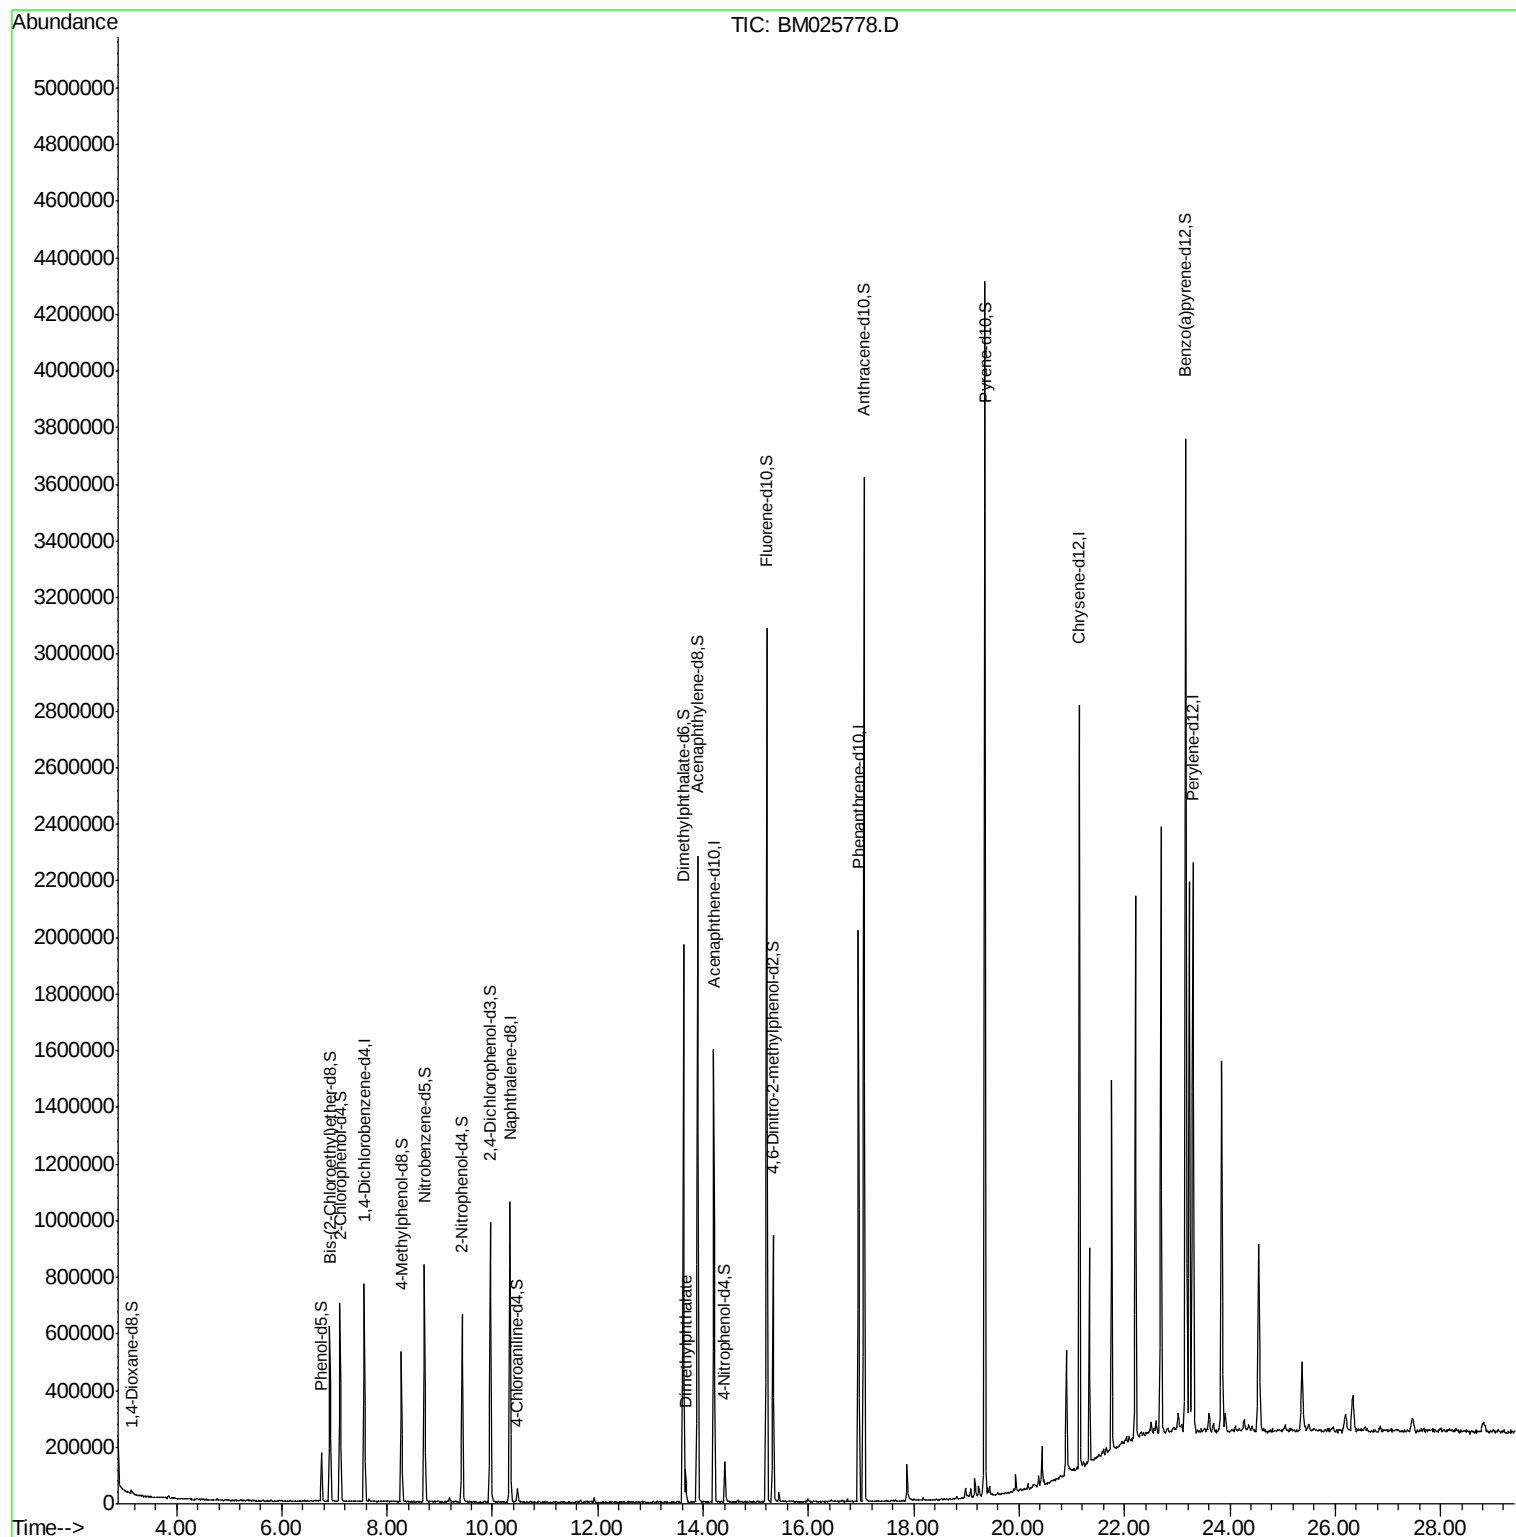

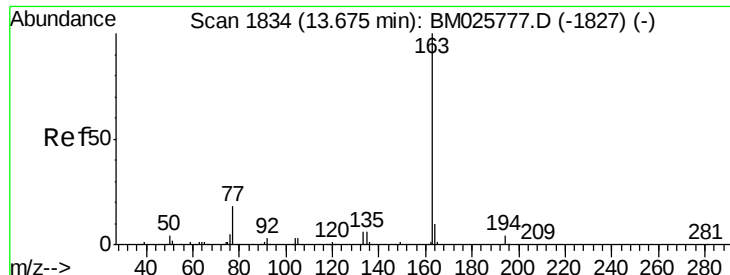

#45

Dimethylphthalate

Concen: 1.663 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BM025778.D

Acq: 25 Mar 2020 21:19

Instrument :

BNA_M

ClientSampleId :

C0DA4


Tot Ion:163 Resp: 70135

Ion Ratio Lower Upper

163 100

194 3.8 3.5 5.3

164 10.1 8.2 12.4

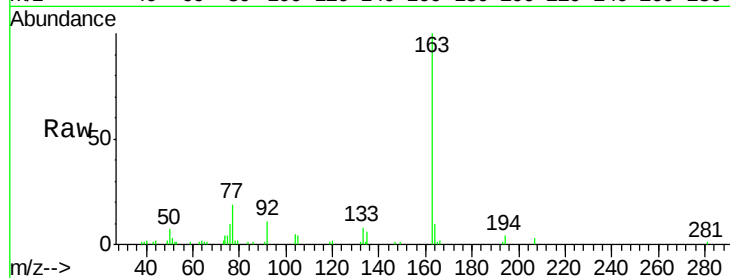

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

