

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025725.D
 Acq On : 24 Mar 2020 12:18
 Operator : CG/JU
 Sample : L1940-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	41	43	52	rVB6	11495	22302	0.41%	0.054%
2	3.852	161	164	167	rVB5	10342	11479	0.21%	0.028%
3	6.246	570	571	579	rVB6	4049	6415	0.12%	0.016%
4	6.757	653	658	667	rVB	165022	250061	4.64%	0.604%
5	6.916	679	685	697	rVB	502992	750499	13.92%	1.814%
6	7.110	712	718	725	rBV	572013	877173	16.27%	2.120%
7	7.569	789	796	805	rBV	621855	961857	17.84%	2.324%
8	7.922	852	856	860	rVB6	4035	6080	0.11%	0.015%
9	8.281	910	917	925	rBV	413617	648491	12.03%	1.567%
10	8.710	984	990	999	rBV	621581	1007559	18.69%	2.435%
11	9.187	1067	1071	1078	rVB2	14653	25288	0.47%	0.061%
12	9.428	1106	1112	1120	rBV	502103	793117	14.71%	1.917%
13	9.963	1196	1203	1215	rBV	767681	1229683	22.81%	2.972%
14	10.204	1240	1244	1248	rVB5	7728	10596	0.20%	0.026%
15	10.339	1260	1267	1276	rVB	794359	1300649	24.13%	3.143%
16	10.486	1289	1292	1297	rBV4	5276	9022	0.17%	0.022%
17	11.681	1489	1495	1501	rVB2	12365	20778	0.39%	0.050%
18	11.933	1533	1538	1542	rBV	12633	16639	0.31%	0.040%
19	13.010	1717	1721	1725	rBV5	3635	5801	0.11%	0.014%
20	13.627	1820	1826	1832	rBV	1640047	2119014	39.31%	5.121%
21	13.675	1832	1834	1842	rVB2	26945	37054	0.69%	0.090%
22	13.898	1864	1872	1881	rBV	1761409	2432987	45.13%	5.880%
23	14.210	1918	1925	1932	rVB	1231957	1739974	32.27%	4.205%
24	14.416	1955	1960	1971	rBV	134783	208779	3.87%	0.505%
25	15.210	2088	2095	2104	rBV	2333312	3290791	61.04%	7.953%
26	15.327	2110	2115	2127	rBV	725513	992409	18.41%	2.398%
27	15.451	2129	2136	2140	rVB2	22855	30654	0.57%	0.074%
28	15.992	2225	2228	2232	rVV4	8607	10632	0.20%	0.026%
29	16.745	2351	2356	2363	rVB4	6107	12159	0.23%	0.029%
30	16.957	2385	2392	2399	rBV	1568417	2150317	39.89%	5.197%
31	17.051	2401	2408	2420	rBV	2748138	3822407	70.90%	9.238%
32	17.874	2545	2548	2553	rBV5	17813	25375	0.47%	0.061%
33	18.739	2693	2695	2702	rVB7	3792	6932	0.13%	0.017%
34	18.986	2733	2737	2741	rVV	27824	34115	0.63%	0.082%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025725.D
 Acq On : 24 Mar 2020 12:18
 Operator : CG/JU
 Sample : L1940-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	19.162	2765	2767	2772	rBV6	8597	11569	0.21%	0.028%
36	19.239	2776	2780	2784	rVB	21598	28243	0.52%	0.068%
37	19.351	2793	2799	2806	rBV	3546038	4607221	85.46%	11.134%
38	20.886	3057	3060	3066	rBV6	38337	53428	0.99%	0.129%
39	21.145	3099	3104	3111	rBV	2314072	2831499	52.52%	6.843%
40	21.756	3206	3208	3214	rVB5	36444	44740	0.83%	0.108%
41	22.203	3282	3284	3288	rVB	62181	62985	1.17%	0.152%
42	22.692	3364	3367	3373	rVB2	95024	128085	2.38%	0.310%
43	23.162	3440	3447	3455	rBV	3181616	5391137	100.00%	13.029%
44	23.233	3456	3459	3463	rVV	113163	159643	2.96%	0.386%
45	23.297	3463	3470	3481	rVB	1734147	3053841	56.65%	7.380%
46	23.844	3560	3563	3573	rVB2	87104	139743	2.59%	0.338%


Sum of corrected areas: 41379222

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025725.D
Acq On : 24 Mar 2020 12:18
Operator : CG/JU
Sample : L1940-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

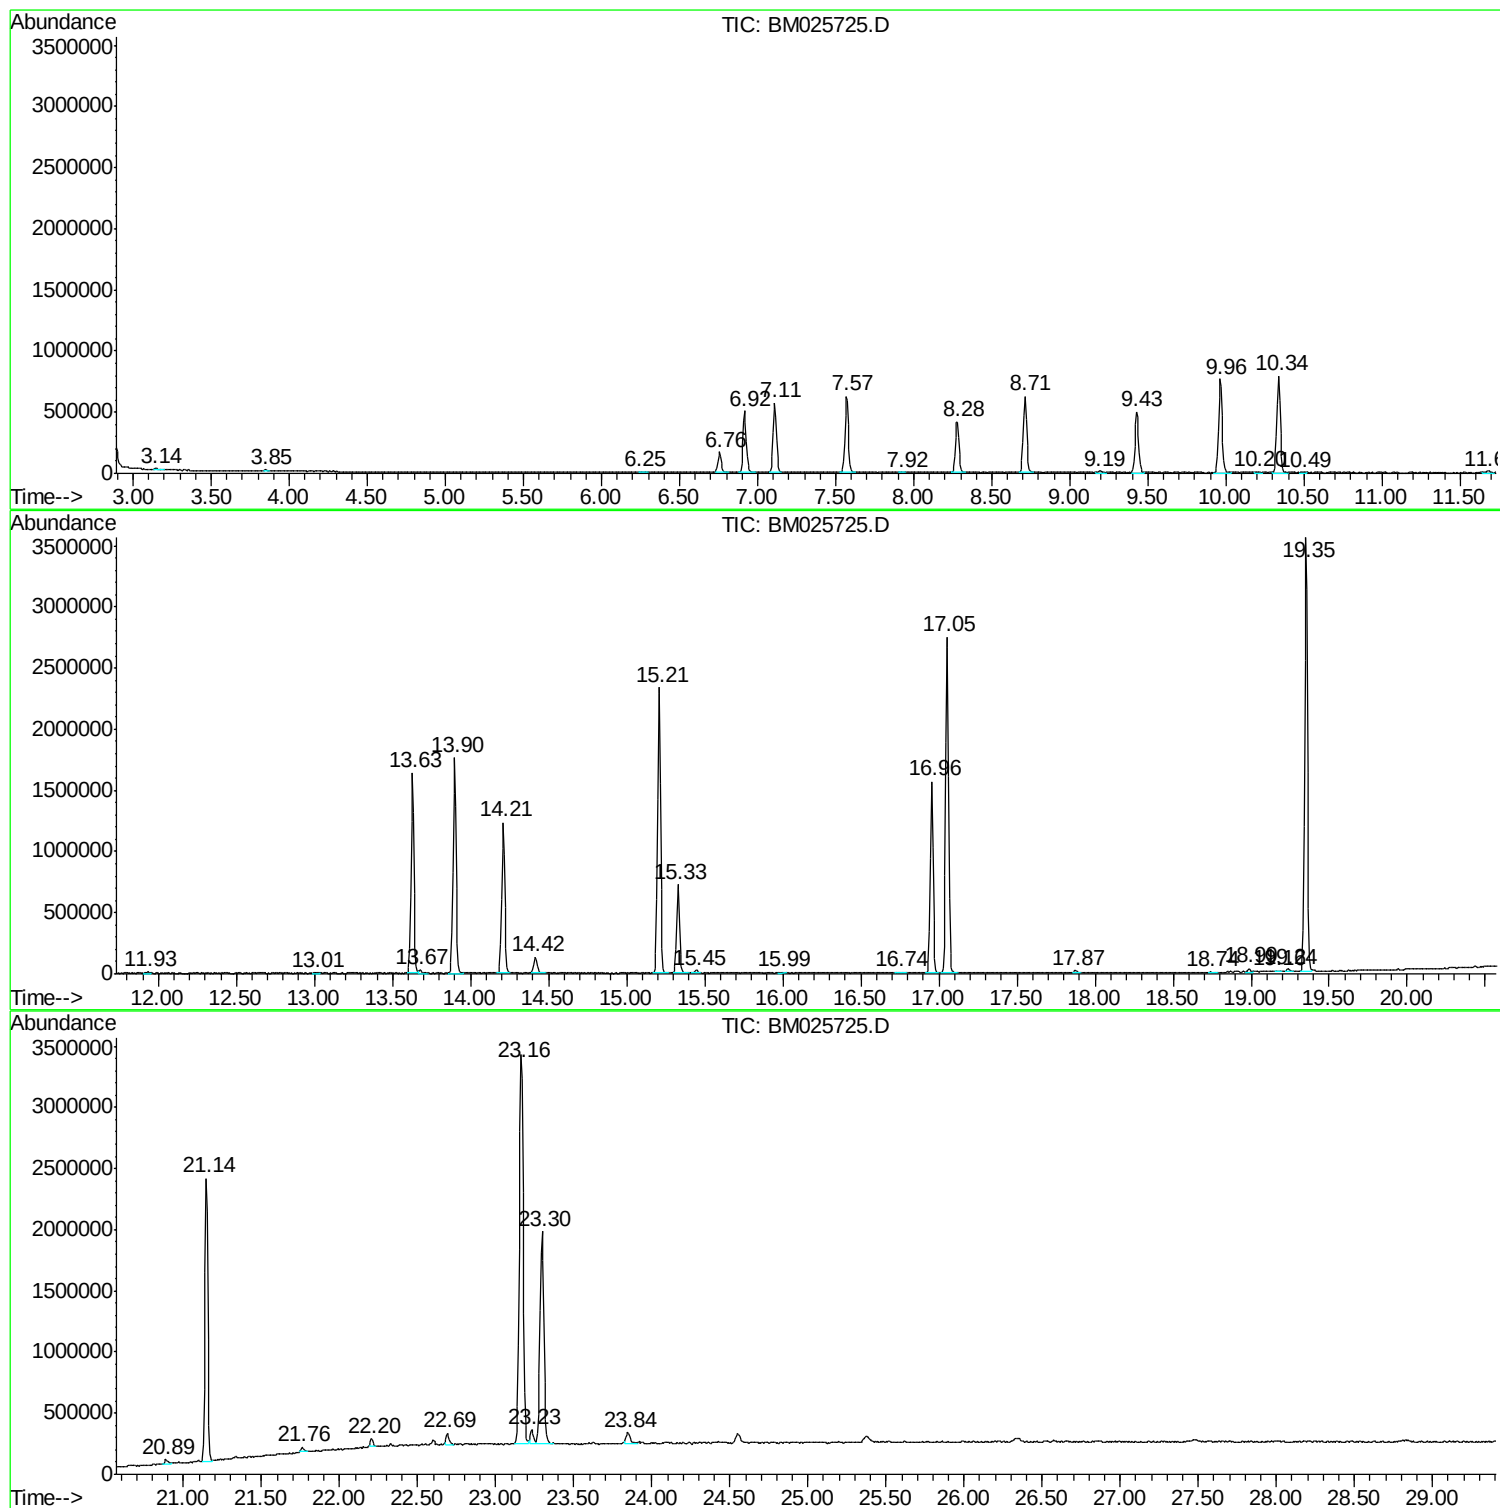

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025725.D
Acq On : 24 Mar 2020 12:18
Operator : CG/JU
Sample : L1940-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025725.D
Acq On : 24 Mar 2020 12:18
Operator : CG/JU
Sample : L1940-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc