

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025726.D
 Acq On : 24 Mar 2020 12:54
 Operator : CG/JU
 Sample : L1940-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	41	44	50	rVB3	10779	17066	0.32%	0.040%
2	3.851	159	164	170	rVB6	10106	17958	0.33%	0.042%
3	6.757	652	658	666	rBV2	177631	286534	5.33%	0.678%
4	6.916	679	685	695	rBV	503094	757644	14.09%	1.792%
5	7.110	711	718	725	rBV	602649	908819	16.90%	2.149%
6	7.569	789	796	805	rBV	623450	968912	18.02%	2.292%
7	7.657	807	811	819	rVB4	10169	16134	0.30%	0.038%
8	8.275	910	916	925	rBV	435909	688649	12.80%	1.629%
9	8.710	984	990	1001	rVB	633841	1017359	18.92%	2.406%
10	9.192	1067	1072	1078	rVB2	29659	44361	0.82%	0.105%
11	9.428	1106	1112	1121	rBV	503747	795160	14.78%	1.881%
12	9.963	1196	1203	1211	rBV	790818	1256074	23.35%	2.971%
13	10.339	1258	1267	1275	rBV	791574	1329516	24.72%	3.144%
14	10.480	1285	1291	1301	rBV3	42007	76554	1.42%	0.181%
15	11.680	1489	1495	1500	rBV2	14446	21309	0.40%	0.050%
16	11.939	1533	1539	1543	rVB3	10602	17947	0.33%	0.042%
17	13.015	1717	1722	1727	rBV5	25081	38510	0.72%	0.091%
18	13.057	1727	1729	1733	rVB5	5060	6397	0.12%	0.015%
19	13.210	1752	1755	1759	rVB3	9132	11750	0.22%	0.028%
20	13.627	1820	1826	1831	rBV	1529963	2032237	37.79%	4.807%
21	13.674	1831	1834	1844	rVB	186559	247131	4.60%	0.584%
22	13.898	1866	1872	1881	rBV	1709149	2419952	45.00%	5.724%
23	14.210	1918	1925	1932	rVB	1239622	1788587	33.26%	4.230%
24	14.415	1954	1960	1972	rBV	145311	227133	4.22%	0.537%
25	15.209	2088	2095	2102	rBV	2312237	3216322	59.80%	7.607%
26	15.327	2110	2115	2125	rBV	710855	977496	18.18%	2.312%
27	15.445	2130	2135	2141	rVB2	22366	31572	0.59%	0.075%
28	15.992	2225	2228	2234	rVB3	7845	10774	0.20%	0.025%
29	16.745	2352	2356	2360	rVB4	6116	10665	0.20%	0.025%
30	16.956	2386	2392	2398	rBV	1610087	2209742	41.09%	5.226%
31	17.056	2402	2409	2417	rBV	2780685	3844434	71.48%	9.093%
32	17.874	2544	2548	2554	rBV2	52078	65527	1.22%	0.155%
33	17.927	2556	2557	2562	rVB4	5403	7905	0.15%	0.019%
34	18.986	2733	2737	2741	rBV	23112	27784	0.52%	0.066%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025726.D
Acq On : 24 Mar 2020 12:54
Operator : CG/JU
Sample : L1940-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D90

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Title : SVOA CALIBRATION

35	19.162	2763	2767	2770	rBV5	12046	17021	0.32%	0.040%
36	19.239	2776	2780	2786	rVB	21935	29777	0.55%	0.070%
37	19.350	2793	2799	2808	rBV	3526961	4666690	86.77%	11.037%
38	20.886	3057	3060	3067	rBV2	179368	245593	4.57%	0.581%
39	21.144	3099	3104	3111	rBV	2326033	2828388	52.59%	6.690%
40	21.333	3134	3136	3139	rVB3	26180	24199	0.45%	0.057%
41	21.762	3206	3209	3213	rVB5	52519	65365	1.22%	0.155%
42	22.203	3282	3284	3288	rVB	68290	69778	1.30%	0.165%
43	22.691	3364	3367	3373	rVB	108436	141273	2.63%	0.334%
44	23.162	3440	3447	3455	rBV	3140019	5378236	100.00%	12.720%
45	23.232	3456	3459	3463	rVV2	143287	210520	3.91%	0.498%
46	23.297	3464	3470	3480	rVB	1711233	3040792	56.54%	7.192%
47	23.844	3560	3563	3569	rVB3	115772	169410	3.15%	0.401%


Sum of corrected areas: 42280956

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025726.D
Acq On : 24 Mar 2020 12:54
Operator : CG/JU
Sample : L1940-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

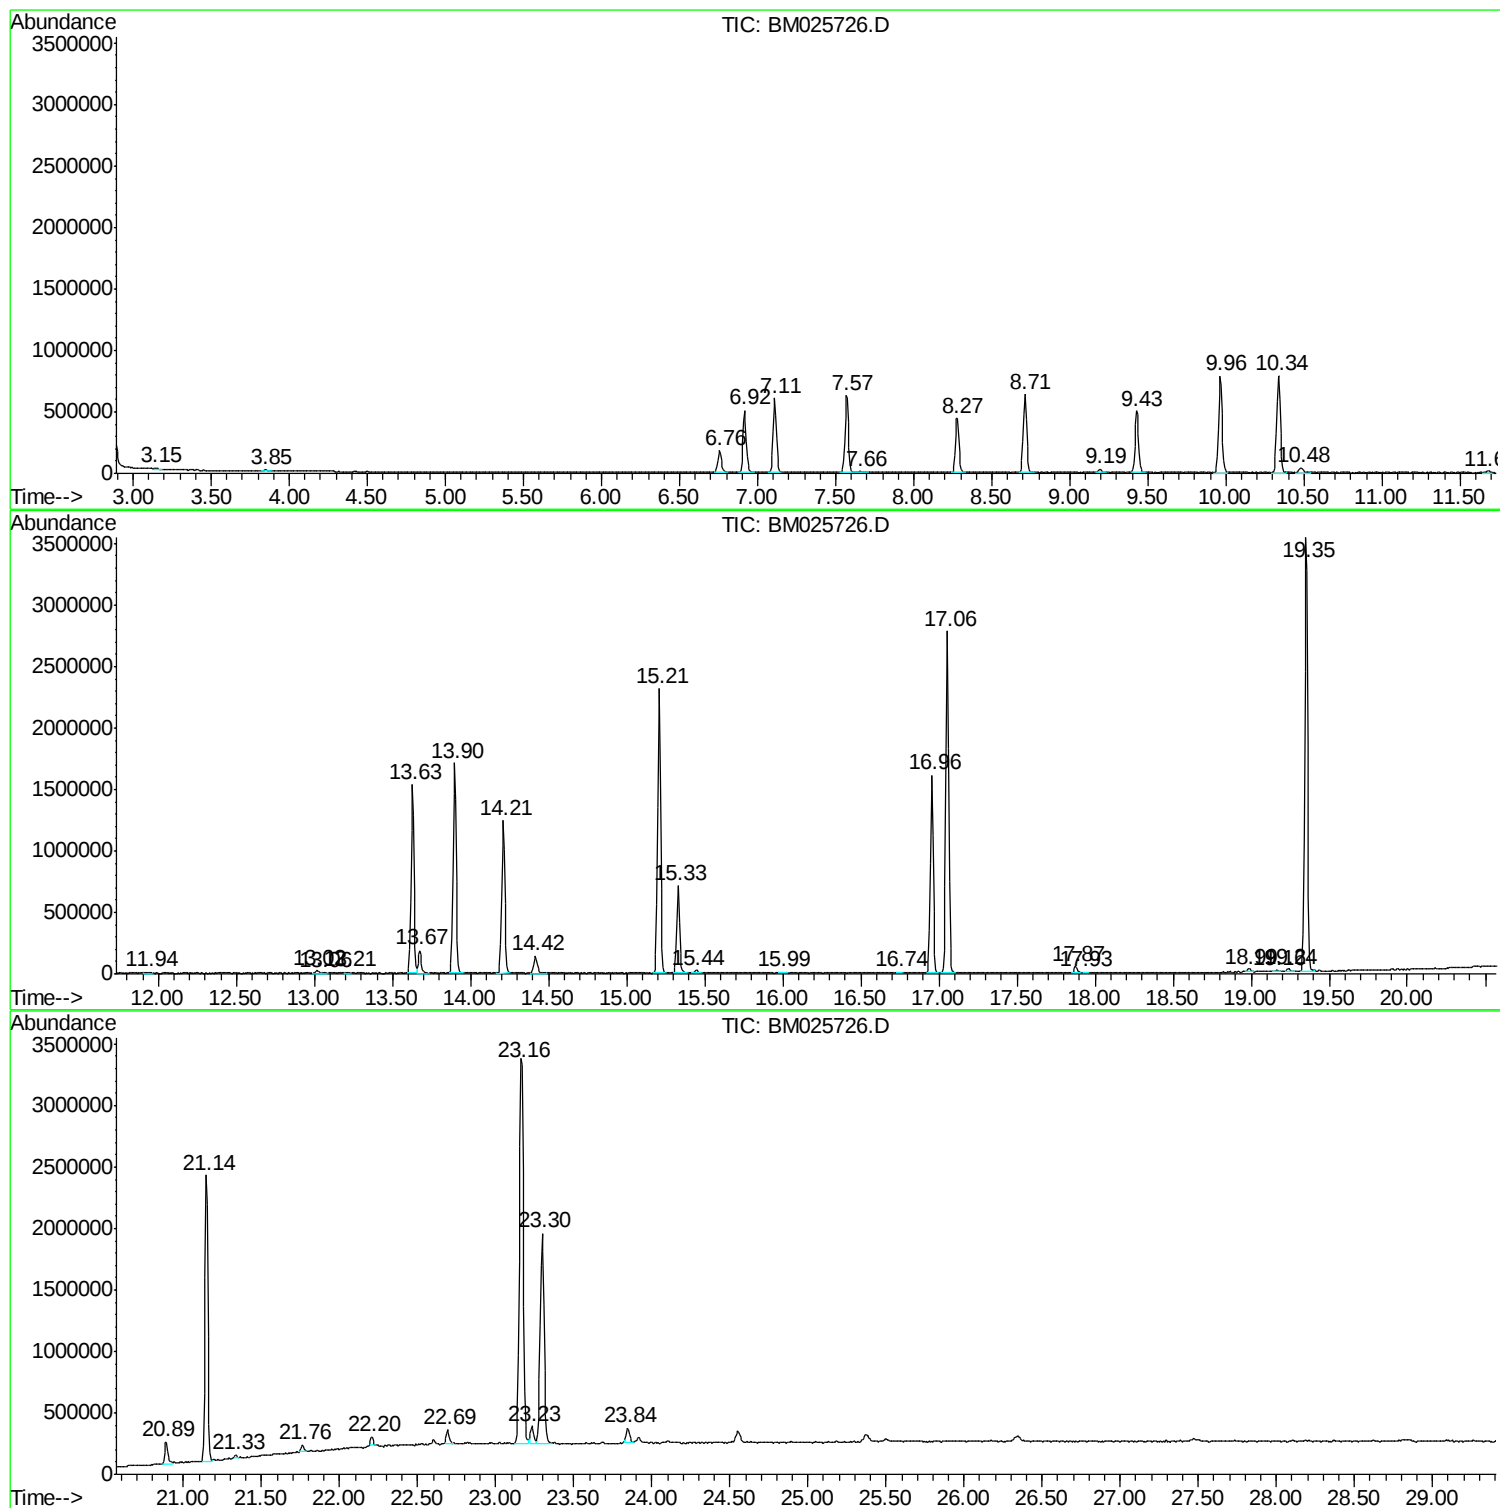

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025726.D
Acq On : 24 Mar 2020 12:54
Operator : CG/JU
Sample : L1940-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025726.D
Acq On : 24 Mar 2020 12:54
Operator : CG/JU
Sample : L1940-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc