

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025728.D
 Acq On : 24 Mar 2020 14:06
 Operator : CG/JU
 Sample : L1940-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	41	43	49	rVB3	12362	17069	0.29%	0.037%
2	3.852	160	164	168	rBV2	9013	10839	0.18%	0.023%
3	6.757	651	658	666	rVB	160430	249739	4.23%	0.541%
4	6.916	679	685	701	rVB	567294	860903	14.58%	1.866%
5	7.110	711	718	727	rVB	632247	968591	16.41%	2.099%
6	7.569	790	796	805	rVB	653700	995750	16.87%	2.158%
7	8.275	910	916	927	rBV	445135	698918	11.84%	1.515%
8	8.710	982	990	1006	rBV	737513	1189788	20.16%	2.578%
9	9.187	1066	1071	1078	rVB4	14856	26862	0.46%	0.058%
10	9.428	1106	1112	1122	rBV	595748	932940	15.81%	2.022%
11	9.963	1197	1203	1212	rBV	894682	1428187	24.20%	3.095%
12	10.169	1233	1238	1240	rBV4	5743	8649	0.15%	0.019%
13	10.339	1257	1267	1274	rBV	807847	1362288	23.08%	2.952%
14	10.492	1288	1293	1300	rVB2	6768	13279	0.22%	0.029%
15	11.098	1391	1396	1400	rBV4	9436	15060	0.26%	0.033%
16	11.675	1488	1494	1500	rBV3	17230	28752	0.49%	0.062%
17	11.933	1533	1538	1543	rBV	13821	22627	0.38%	0.049%
18	13.016	1715	1722	1729	rVB3	46031	68292	1.16%	0.148%
19	13.210	1750	1755	1761	rVB2	22326	28941	0.49%	0.063%
20	13.627	1820	1826	1834	rBV	1847922	2424969	41.08%	5.255%
21	13.698	1834	1838	1842	rVB3	6937	9266	0.16%	0.020%
22	13.898	1865	1872	1883	rBV	2058420	2896363	49.07%	6.277%
23	14.210	1919	1925	1932	rVB	1317691	1867212	31.63%	4.046%
24	14.416	1955	1960	1968	rBV	128863	196582	3.33%	0.426%
25	15.210	2088	2095	2103	rBV	2724540	3784667	64.12%	8.202%
26	15.333	2109	2116	2128	rBV	835046	1149119	19.47%	2.490%
27	15.451	2130	2136	2140	rVB	25747	34340	0.58%	0.074%
28	15.992	2224	2228	2233	rVB6	8955	11817	0.20%	0.026%
29	16.745	2350	2356	2362	rBV4	5026	10881	0.18%	0.024%
30	16.957	2385	2392	2399	rBV	1726345	2300583	38.97%	4.986%
31	17.057	2402	2409	2420	rVB	3127819	4306991	72.97%	9.334%
32	17.880	2544	2549	2552	rVB4	15324	18227	0.31%	0.039%
33	17.933	2554	2558	2563	rBV4	7570	11925	0.20%	0.026%
34	18.986	2733	2737	2743	rVB	30312	36591	0.62%	0.079%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025728.D
Acq On : 24 Mar 2020 14:06
Operator : CG/JU
Sample : L1940-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D92

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Title : SVOA CALIBRATION

35	19.168	2763	2768	2772	rBV5	8727	16709	0.28%	0.036%
36	19.239	2776	2780	2787	rVV	25503	34975	0.59%	0.076%
37	19.351	2793	2799	2806	rBV	3781138	5194495	88.00%	11.257%
38	20.898	3060	3062	3065	rBV3	21653	16314	0.28%	0.035%
39	21.145	3099	3104	3111	rBV	2299711	2926682	49.58%	6.342%
40	21.339	3134	3137	3142	rVB3	40825	43610	0.74%	0.095%
41	21.762	3205	3209	3213	rBV	82851	97381	1.65%	0.211%
42	22.209	3281	3285	3288	rBV	123516	149327	2.53%	0.324%
43	22.692	3363	3367	3373	rVB	156179	207417	3.51%	0.449%
44	23.168	3441	3448	3454	rBV	3492775	5902760	100.00%	12.792%
45	23.233	3455	3459	3463	rVV	163482	256586	4.35%	0.556%
46	23.297	3464	3470	3481	rVB	1770371	3109795	52.68%	6.739%
47	23.844	3560	3563	3569	rVB2	133129	202028	3.42%	0.438%


Sum of corrected areas: 46145086

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025728.D
Acq On : 24 Mar 2020 14:06
Operator : CG/JU
Sample : L1940-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D92

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

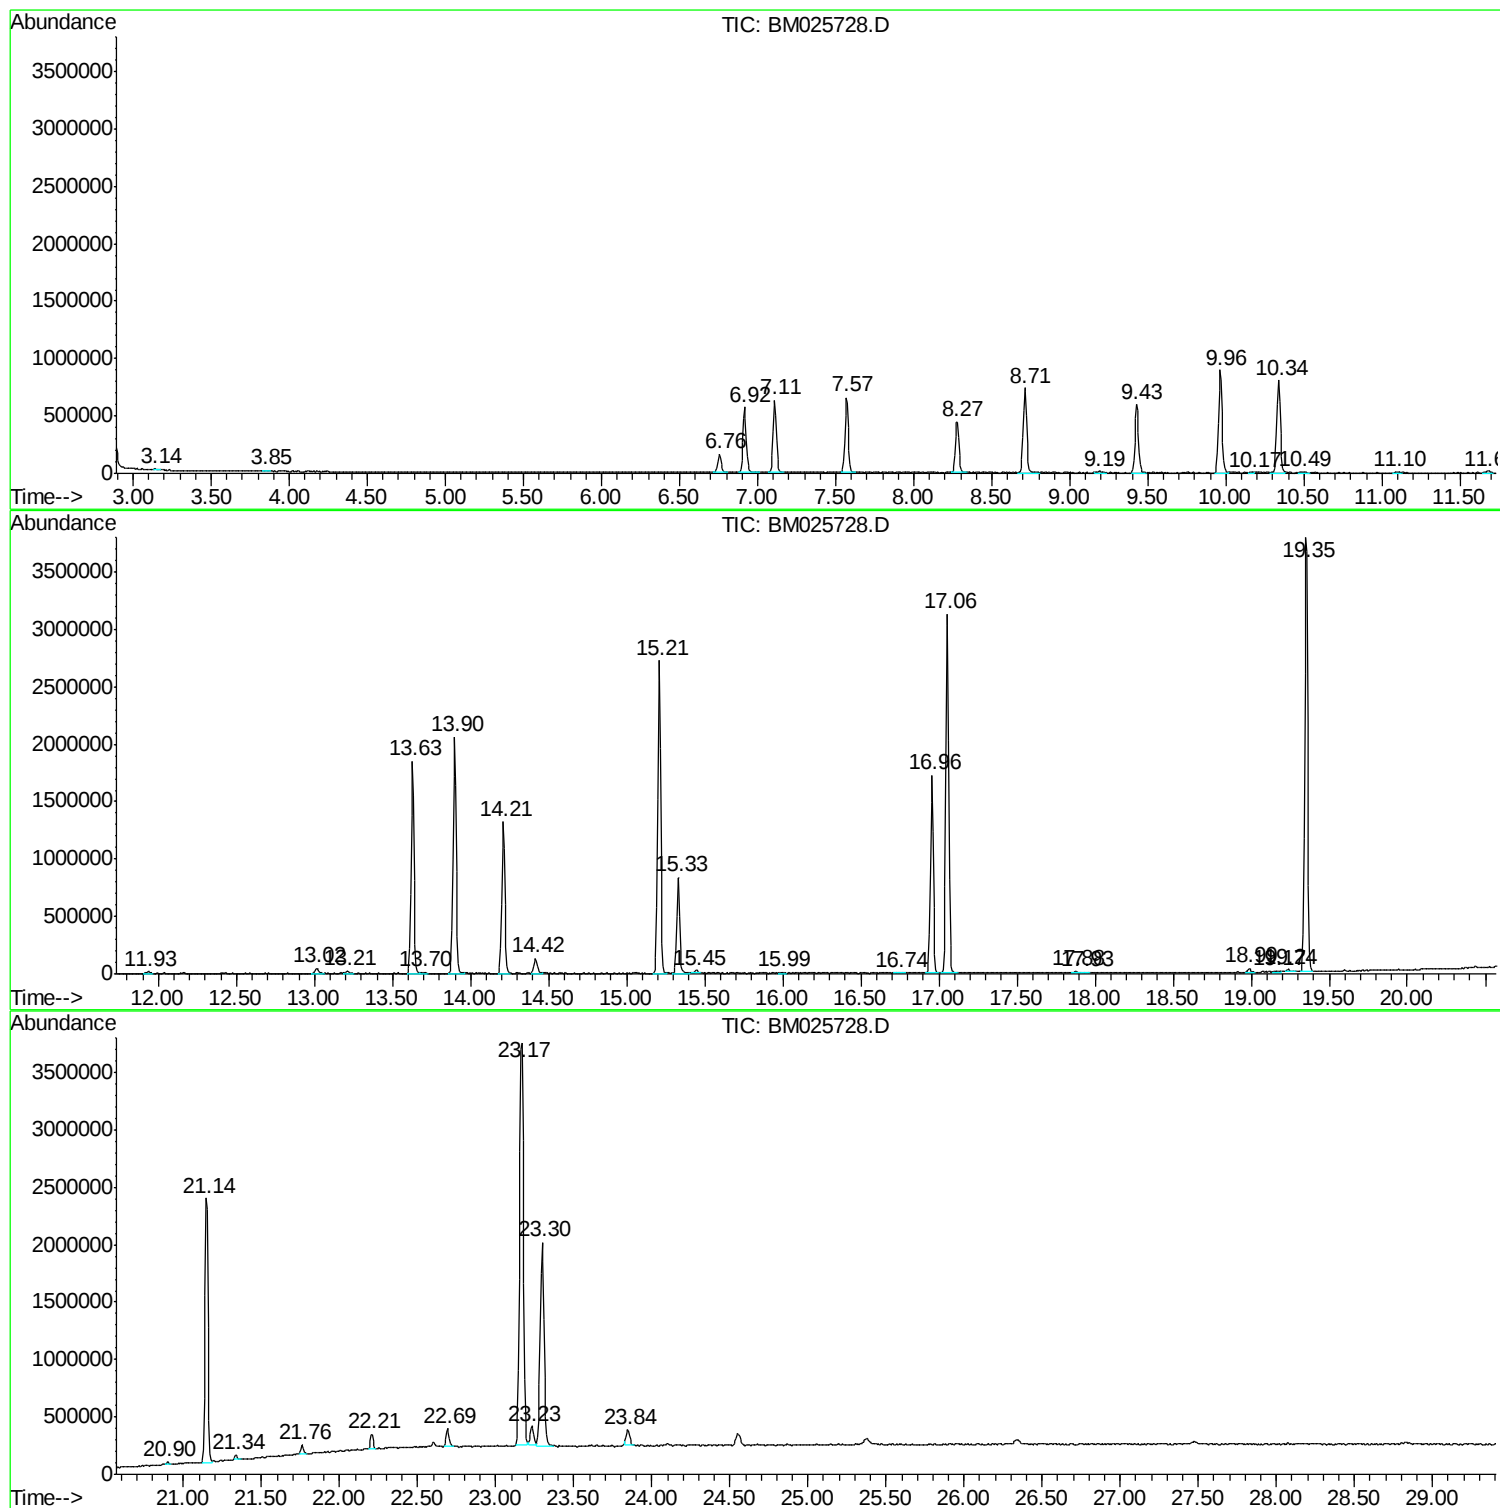

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025728.D
Acq On : 24 Mar 2020 14:06
Operator : CG/JU
Sample : L1940-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D92

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025728.D
Acq On : 24 Mar 2020 14:06
Operator : CG/JU
Sample : L1940-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D92

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc