

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025731.D
 Acq On : 24 Mar 2020 15:54
 Operator : CG/JU
 Sample : L1940-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	41	44	49	rVB4	11082	14293	0.30%	0.037%
2	3.769	147	150	154	rVB4	4396	5484	0.12%	0.014%
3	3.846	160	163	168	rVB3	10507	13304	0.28%	0.035%
4	4.775	318	321	326	rVB6	3900	5544	0.12%	0.014%
5	6.381	590	594	602	rVB7	2410	4921	0.10%	0.013%
6	6.757	651	658	664	rBV	144996	219600	4.61%	0.570%
7	6.916	679	685	698	rBV	492982	755344	15.87%	1.962%
8	7.110	710	718	727	rVV	570302	860562	18.08%	2.235%
9	7.569	790	796	807	rVB	621332	959241	20.15%	2.491%
10	8.275	909	916	924	rBV	389638	612033	12.86%	1.589%
11	8.710	981	990	999	rBV	614032	1000197	21.01%	2.597%
12	9.192	1065	1072	1076	rVB5	10381	13974	0.29%	0.036%
13	9.428	1106	1112	1121	rVB	491305	767836	16.13%	1.994%
14	9.963	1196	1203	1217	rBV	750257	1207677	25.37%	3.136%
15	10.339	1258	1267	1273	rBV	792997	1306078	27.44%	3.392%
16	10.480	1286	1291	1299	rVB2	33952	56614	1.19%	0.147%
17	11.680	1492	1495	1500	rVB4	6603	8257	0.17%	0.021%
18	11.939	1534	1539	1544	rVB3	11107	16268	0.34%	0.042%
19	12.027	1550	1554	1561	rBV5	15027	24510	0.51%	0.064%
20	13.016	1716	1722	1729	rBV2	57084	78083	1.64%	0.203%
21	13.210	1750	1755	1760	rVB2	16685	24877	0.52%	0.065%
22	13.627	1820	1826	1832	rBV	1460105	1939815	40.75%	5.038%
23	13.674	1832	1834	1841	rVB	11261	14320	0.30%	0.037%
24	13.898	1865	1872	1881	rBV	1642916	2285499	48.01%	5.935%
25	13.968	1881	1884	1888	rVB4	6355	8232	0.17%	0.021%
26	14.210	1918	1925	1936	rVB	1219628	1733905	36.42%	4.503%
27	14.415	1954	1960	1968	rBV2	109773	174330	3.66%	0.453%
28	15.210	2088	2095	2102	rBV	2213291	3010288	63.24%	7.818%
29	15.327	2107	2115	2126	rBV	659889	887231	18.64%	2.304%
30	15.445	2131	2135	2140	rVB2	22157	30835	0.65%	0.080%
31	15.992	2223	2228	2232	rBV4	6637	8867	0.19%	0.023%
32	16.739	2352	2355	2356	rBV2	5834	5869	0.12%	0.015%
33	16.956	2386	2392	2399	rVB	1523462	2068595	43.45%	5.372%
34	17.057	2402	2409	2422	rVV	2488833	3445522	72.38%	8.948%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025731.D
 Acq On : 24 Mar 2020 15:54
 Operator : CG/JU
 Sample : L1940-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	17.874	2543	2548	2553	rBV5	20370	26308	0.55%	0.068%
36	17.939	2553	2559	2564	rVV	55637	78815	1.66%	0.205%
37	18.145	2591	2594	2597	rBV4	4139	5034	0.11%	0.013%
38	18.186	2597	2601	2606	rVV6	5291	8261	0.17%	0.021%
39	18.756	2696	2698	2703	rVB5	4082	6121	0.13%	0.016%
40	18.986	2733	2737	2743	rBV2	27057	41294	0.87%	0.107%
41	19.086	2751	2754	2755	rBV3	5385	5571	0.12%	0.014%
42	19.162	2764	2767	2774	rBV6	10497	19648	0.41%	0.051%
43	19.239	2777	2780	2784	rVB	21740	26731	0.56%	0.069%
44	19.350	2793	2799	2807	rBV	3171449	4154713	87.28%	10.790%
45	19.598	2837	2841	2845	rBV7	5163	8242	0.17%	0.021%
46	20.892	3057	3061	3068	rBV8	35179	56504	1.19%	0.147%
47	21.144	3099	3104	3111	rBV	2179052	2660559	55.89%	6.909%
48	22.691	3364	3367	3371	rVB2	89315	106872	2.24%	0.278%
49	23.162	3441	3447	3455	rBV	2810402	4760474	100.00%	12.363%
50	23.233	3456	3459	3464	rVV3	99425	146522	3.08%	0.381%
51	23.297	3464	3470	3480	rVB	1664634	2826565	59.38%	7.341%


Sum of corrected areas: 38506239

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025731.D
Acq On : 24 Mar 2020 15:54
Operator : CG/JU
Sample : L1940-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D96

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

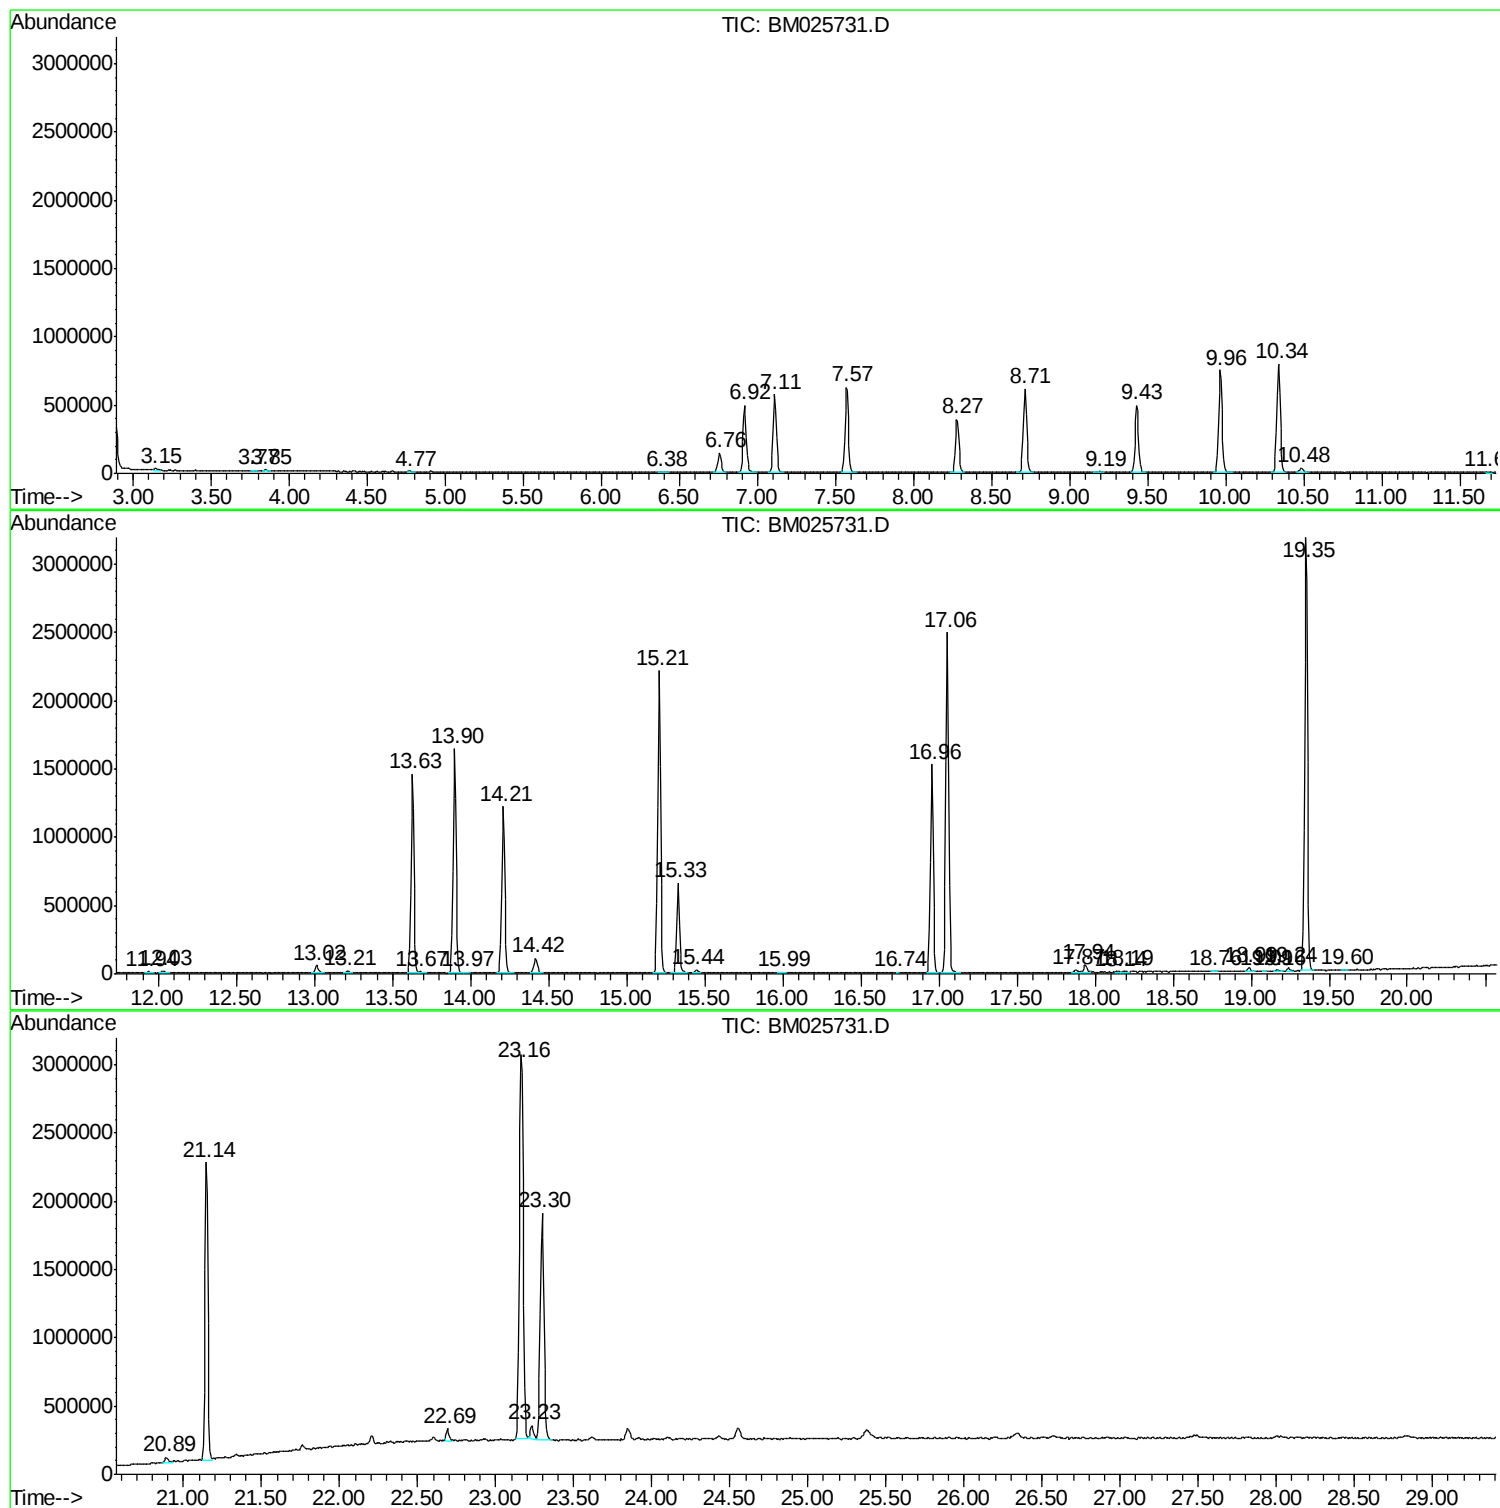

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025731.D
Acq On : 24 Mar 2020 15:54
Operator : CG/JU
Sample : L1940-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D96

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025731.D
Acq On : 24 Mar 2020 15:54
Operator : CG/JU
Sample : L1940-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0D96

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
