

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025737.D
 Acq On : 24 Mar 2020 20:08
 Operator : CG/JU
 Sample : L1940-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	41	44	47	rBV3	7153	9547	0.20%	0.025%
2	3.846	159	163	168	rBV3	9419	13968	0.30%	0.036%
3	6.757	652	658	665	rVB	140874	225410	4.83%	0.580%
4	6.916	679	685	699	rBV	484546	722508	15.48%	1.859%
5	7.110	711	718	725	rBV	544827	835401	17.90%	2.150%
6	7.569	790	796	805	rBV	602994	913354	19.57%	2.350%
7	7.657	807	811	815	rVB	6905	11006	0.24%	0.028%
8	8.275	910	916	929	rBV	405858	626005	13.41%	1.611%
9	8.710	983	990	998	rBV	616408	985790	21.12%	2.537%
10	9.192	1064	1072	1075	rBV2	17180	23727	0.51%	0.061%
11	9.428	1106	1112	1122	rBV	488170	765440	16.40%	1.970%
12	9.963	1196	1203	1215	rBV	771419	1209647	25.92%	3.113%
13	10.334	1259	1266	1274	rBV	781902	1249150	26.76%	3.214%
14	10.481	1286	1291	1300	rBV	36847	63879	1.37%	0.164%
15	11.681	1492	1495	1498	rBV2	6306	7449	0.16%	0.019%
16	11.933	1534	1538	1544	rVB5	11335	18907	0.41%	0.049%
17	13.057	1725	1729	1735	rBV4	2918	4727	0.10%	0.012%
18	13.627	1819	1826	1830	rBV	1502195	2013285	43.13%	5.181%
19	13.675	1830	1834	1841	rVB	240256	328637	7.04%	0.846%
20	13.898	1865	1872	1879	rBV	1704590	2377639	50.94%	6.118%
21	14.145	1911	1914	1917	rBV3	4480	5628	0.12%	0.014%
22	14.210	1919	1925	1934	rVB2	1206462	1697294	36.36%	4.368%
23	14.416	1954	1960	1972	rBV	114119	179380	3.84%	0.462%
24	15.204	2088	2094	2103	rBV	2228806	3136677	67.20%	8.072%
25	15.327	2110	2115	2130	rBV	651393	863763	18.51%	2.223%
26	15.451	2132	2136	2141	rVB2	21345	27511	0.59%	0.071%
27	15.551	2149	2153	2157	rBV5	3118	5152	0.11%	0.013%
28	15.992	2225	2228	2231	rVB2	8489	9928	0.21%	0.026%
29	16.739	2353	2355	2359	rVB3	4066	4701	0.10%	0.012%
30	16.957	2384	2392	2401	rBV	1548285	2058643	44.10%	5.298%
31	17.051	2402	2408	2419	rVV	2556909	3536851	75.77%	9.101%
32	17.586	2494	2499	2501	rBV5	3925	5857	0.13%	0.015%
33	17.874	2545	2548	2555	rBV	39746	51386	1.10%	0.132%
34	18.986	2733	2737	2740	rBV2	25857	28454	0.61%	0.073%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025737.D
Acq On : 24 Mar 2020 20:08
Operator : CG/JU
Sample : L1940-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Title : SVOA CALIBRATION

35	19.080	2750	2753	2755	rBV3	4128	4670	0.10%	0.012%
36	19.168	2764	2768	2772	rBV6	7465	10128	0.22%	0.026%
37	19.239	2776	2780	2784	rVV	20678	23477	0.50%	0.060%
38	19.351	2793	2799	2805	rBV	3249931	4106997	87.99%	10.569%
39	19.939	2897	2899	2904	rVB5	10736	9917	0.21%	0.026%
40	20.409	2977	2979	2981	rBV2	7957	7164	0.15%	0.018%
41	20.439	2981	2984	2987	rVV3	16033	19929	0.43%	0.051%
42	20.892	3057	3061	3067	rBV2	160001	221196	4.74%	0.569%
43	21.145	3099	3104	3113	rBV	2013064	2542240	54.47%	6.542%
44	21.339	3134	3137	3140	rVB2	48247	55072	1.18%	0.142%
45	21.762	3206	3209	3213	rVB2	69751	79242	1.70%	0.204%
46	22.209	3282	3285	3289	rVB2	75979	83613	1.79%	0.215%
47	22.692	3364	3367	3372	rVB	96021	114876	2.46%	0.296%
48	23.162	3441	3447	3455	rVV	2788108	4667648	100.00%	12.011%
49	23.233	3456	3459	3463	rVB2	103730	137737	2.95%	0.354%
50	23.297	3464	3470	3479	rVB	1608317	2759488	59.12%	7.101%


Sum of corrected areas: 38860095

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025737.D
Acq On : 24 Mar 2020 20:08
Operator : CG/JU
Sample : L1940-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

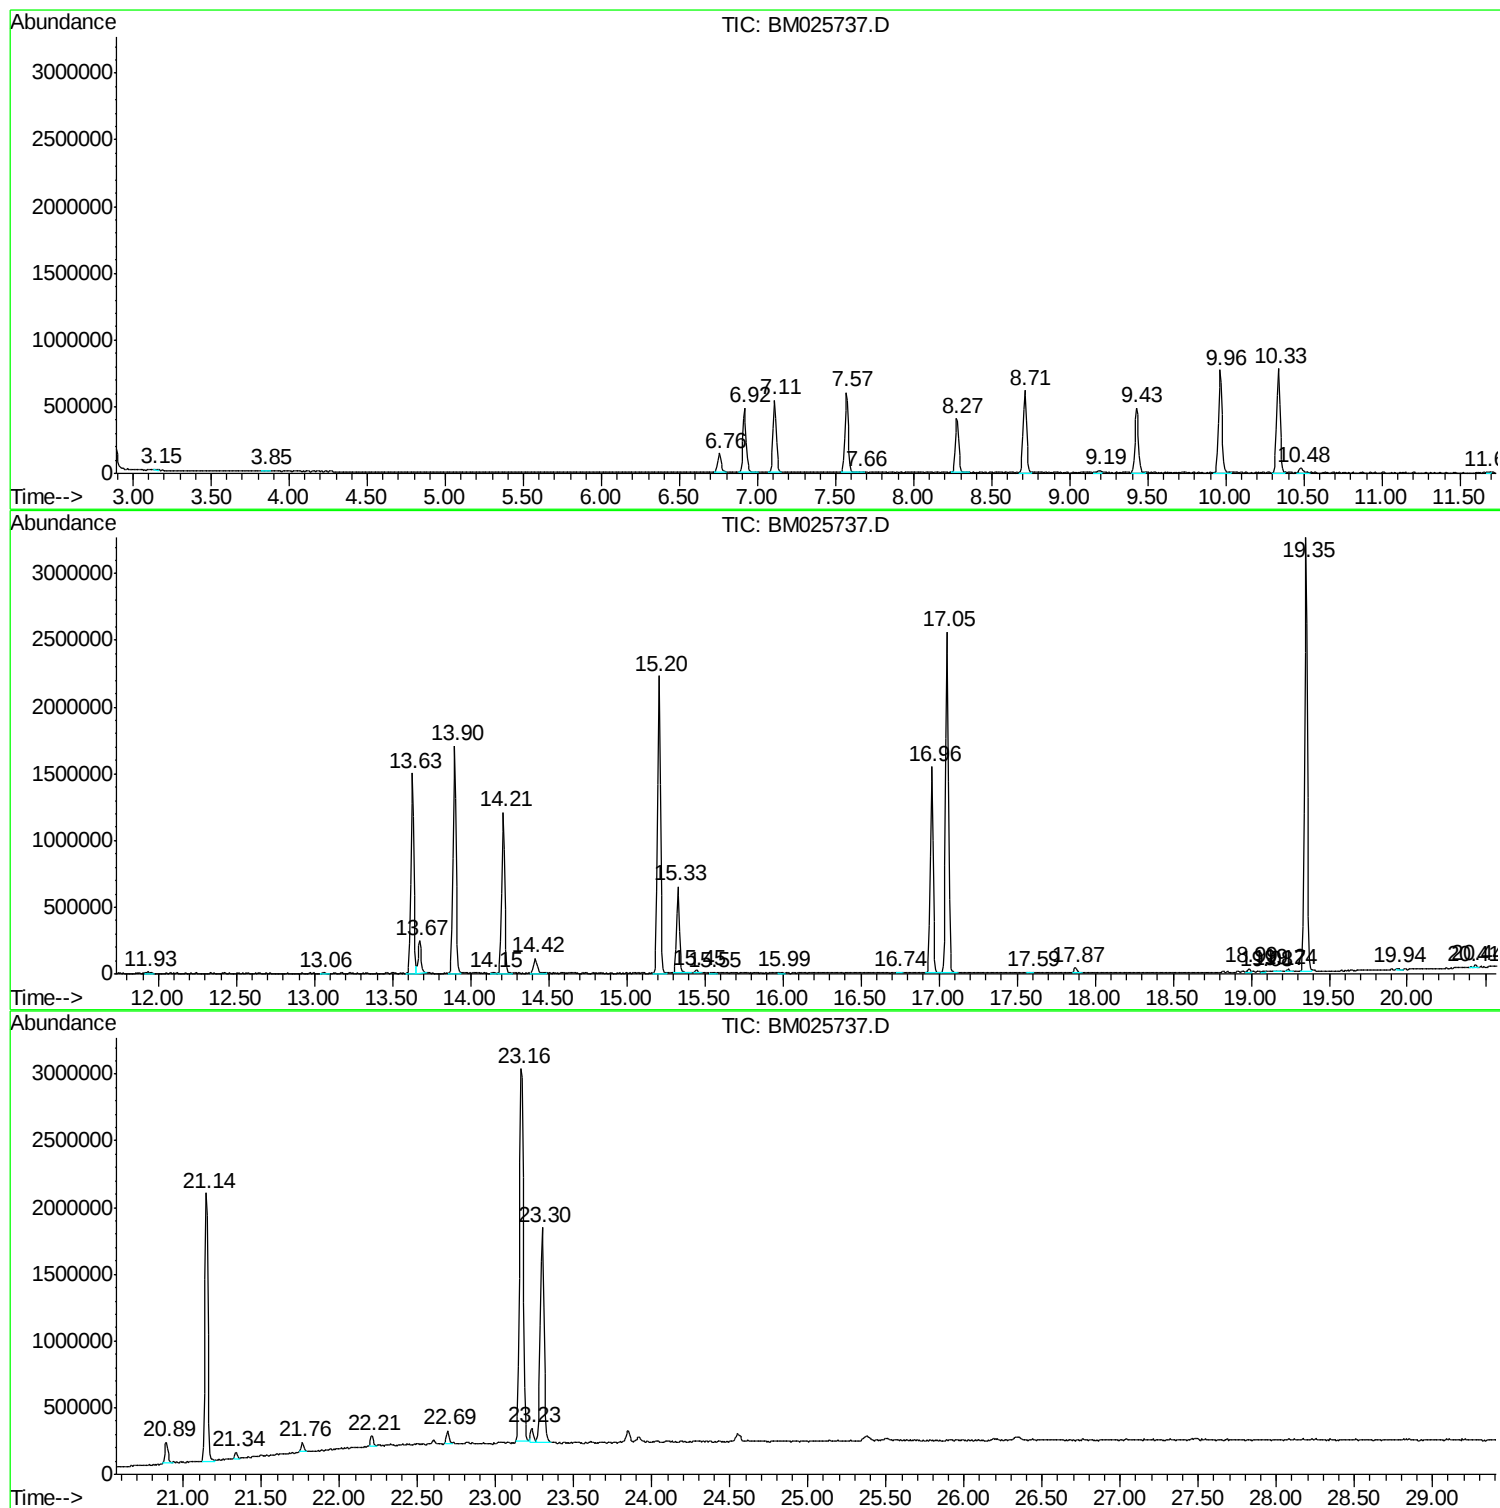

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025737.D
Acq On : 24 Mar 2020 20:08
Operator : CG/JU
Sample : L1940-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025737.D
Acq On : 24 Mar 2020 20:08
Operator : CG/JU
Sample : L1940-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
