

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025738.D
 Acq On : 24 Mar 2020 20:44
 Operator : CG/JU
 Sample : L1940-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	41	44	51	rVB2	12506	20504	0.32%	0.039%
2	3.852	160	164	168	rVB2	9713	13417	0.21%	0.026%
3	6.757	651	658	666	rVB	179161	289464	4.54%	0.553%
4	6.916	678	685	697	rBV	652155	989918	15.54%	1.891%
5	7.110	711	718	727	rBV	732617	1129923	17.74%	2.158%
6	7.569	790	796	807	rVB	742328	1134872	17.82%	2.168%
7	8.275	910	916	925	rBV	540139	825392	12.96%	1.577%
8	8.710	982	990	1000	rBV	843808	1352020	21.23%	2.582%
9	9.175	1064	1069	1077	rVB4	21117	52359	0.82%	0.100%
10	9.428	1105	1112	1126	rVB	686030	1072327	16.84%	2.048%
11	9.963	1196	1203	1216	rBV	1031873	1636861	25.70%	3.126%
12	10.334	1259	1266	1277	rVB	952706	1579934	24.80%	3.018%
13	10.487	1285	1292	1297	rBV2	17164	30963	0.49%	0.059%
14	11.681	1488	1495	1500	rBV2	18483	26205	0.41%	0.050%
15	11.939	1531	1539	1544	rBV2	15835	27596	0.43%	0.053%
16	12.034	1550	1555	1561	rBV6	4085	7607	0.12%	0.015%
17	12.157	1573	1576	1583	rVB5	3892	7556	0.12%	0.014%
18	13.010	1716	1721	1728	rBV	95862	139737	2.19%	0.267%
19	13.210	1750	1755	1760	rVV	50801	74957	1.18%	0.143%
20	13.628	1820	1826	1833	rBV	2083917	2790095	43.80%	5.329%
21	13.692	1833	1837	1842	rVB5	7220	13722	0.22%	0.026%
22	13.898	1865	1872	1879	rBV	2368779	3287420	51.61%	6.279%
23	13.969	1881	1884	1889	rVB4	9546	12420	0.19%	0.024%
24	14.210	1919	1925	1938	rVB2	1548671	2192581	34.42%	4.188%
25	14.416	1952	1960	1974	rBV	155072	245558	3.86%	0.469%
26	15.210	2088	2095	2101	rBV	3024972	4289444	67.34%	8.193%
27	15.327	2109	2115	2130	rBV	960402	1272819	19.98%	2.431%
28	15.445	2131	2135	2140	rVB	31289	40860	0.64%	0.078%
29	15.992	2224	2228	2234	rVB4	10695	16382	0.26%	0.031%
30	16.639	2334	2338	2344	rBV7	4028	7250	0.11%	0.014%
31	16.745	2349	2356	2362	rVB3	7370	13519	0.21%	0.026%
32	16.951	2385	2391	2402	rVB	1901228	2678762	42.06%	5.116%
33	17.051	2402	2408	2419	rBV	3467312	4759535	74.72%	9.091%
34	17.874	2544	2548	2554	rVV	44445	57350	0.90%	0.110%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
 Data File : BM025738.D
 Acq On : 24 Mar 2020 20:44
 Operator : CG/JU
 Sample : L1940-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0DA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Title : SVOA CALIBRATION

35	17.939	2554	2559	2562	rVB4	18324	25714	0.40%	0.049%
36	18.745	2692	2696	2699	rBV5	6082	6553	0.10%	0.013%
37	18.986	2732	2737	2742	rBV	36456	46942	0.74%	0.090%
38	19.163	2765	2767	2770	rBV4	9886	9682	0.15%	0.018%
39	19.233	2776	2779	2784	rVB	26378	34200	0.54%	0.065%
40	19.351	2793	2799	2806	rBV	4374224	5598829	87.90%	10.694%
41	20.886	3056	3060	3066	rBV	153656	200430	3.15%	0.383%
42	21.145	3099	3104	3110	rBV	2671652	3258265	51.15%	6.223%
43	21.333	3134	3136	3140	rVB3	43782	49776	0.78%	0.095%
44	21.762	3205	3209	3215	rBV2	86895	112271	1.76%	0.214%
45	22.203	3281	3284	3289	rBV	140823	166202	2.61%	0.317%
46	22.692	3363	3367	3371	rBV	190021	251514	3.95%	0.480%
47	23.162	3440	3447	3454	rBV	3731159	6369452	100.00%	12.166%
48	23.233	3455	3459	3463	rVV	225062	334485	5.25%	0.639%
49	23.298	3463	3470	3480	rVB	2024688	3525593	55.35%	6.734%
50	23.845	3559	3563	3569	rVB	169373	276576	4.34%	0.528%


Sum of corrected areas: 52355813

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032320\
Data File : BM025738.D
Acq On : 24 Mar 2020 20:44
Operator : CG/JU
Sample : L1940-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

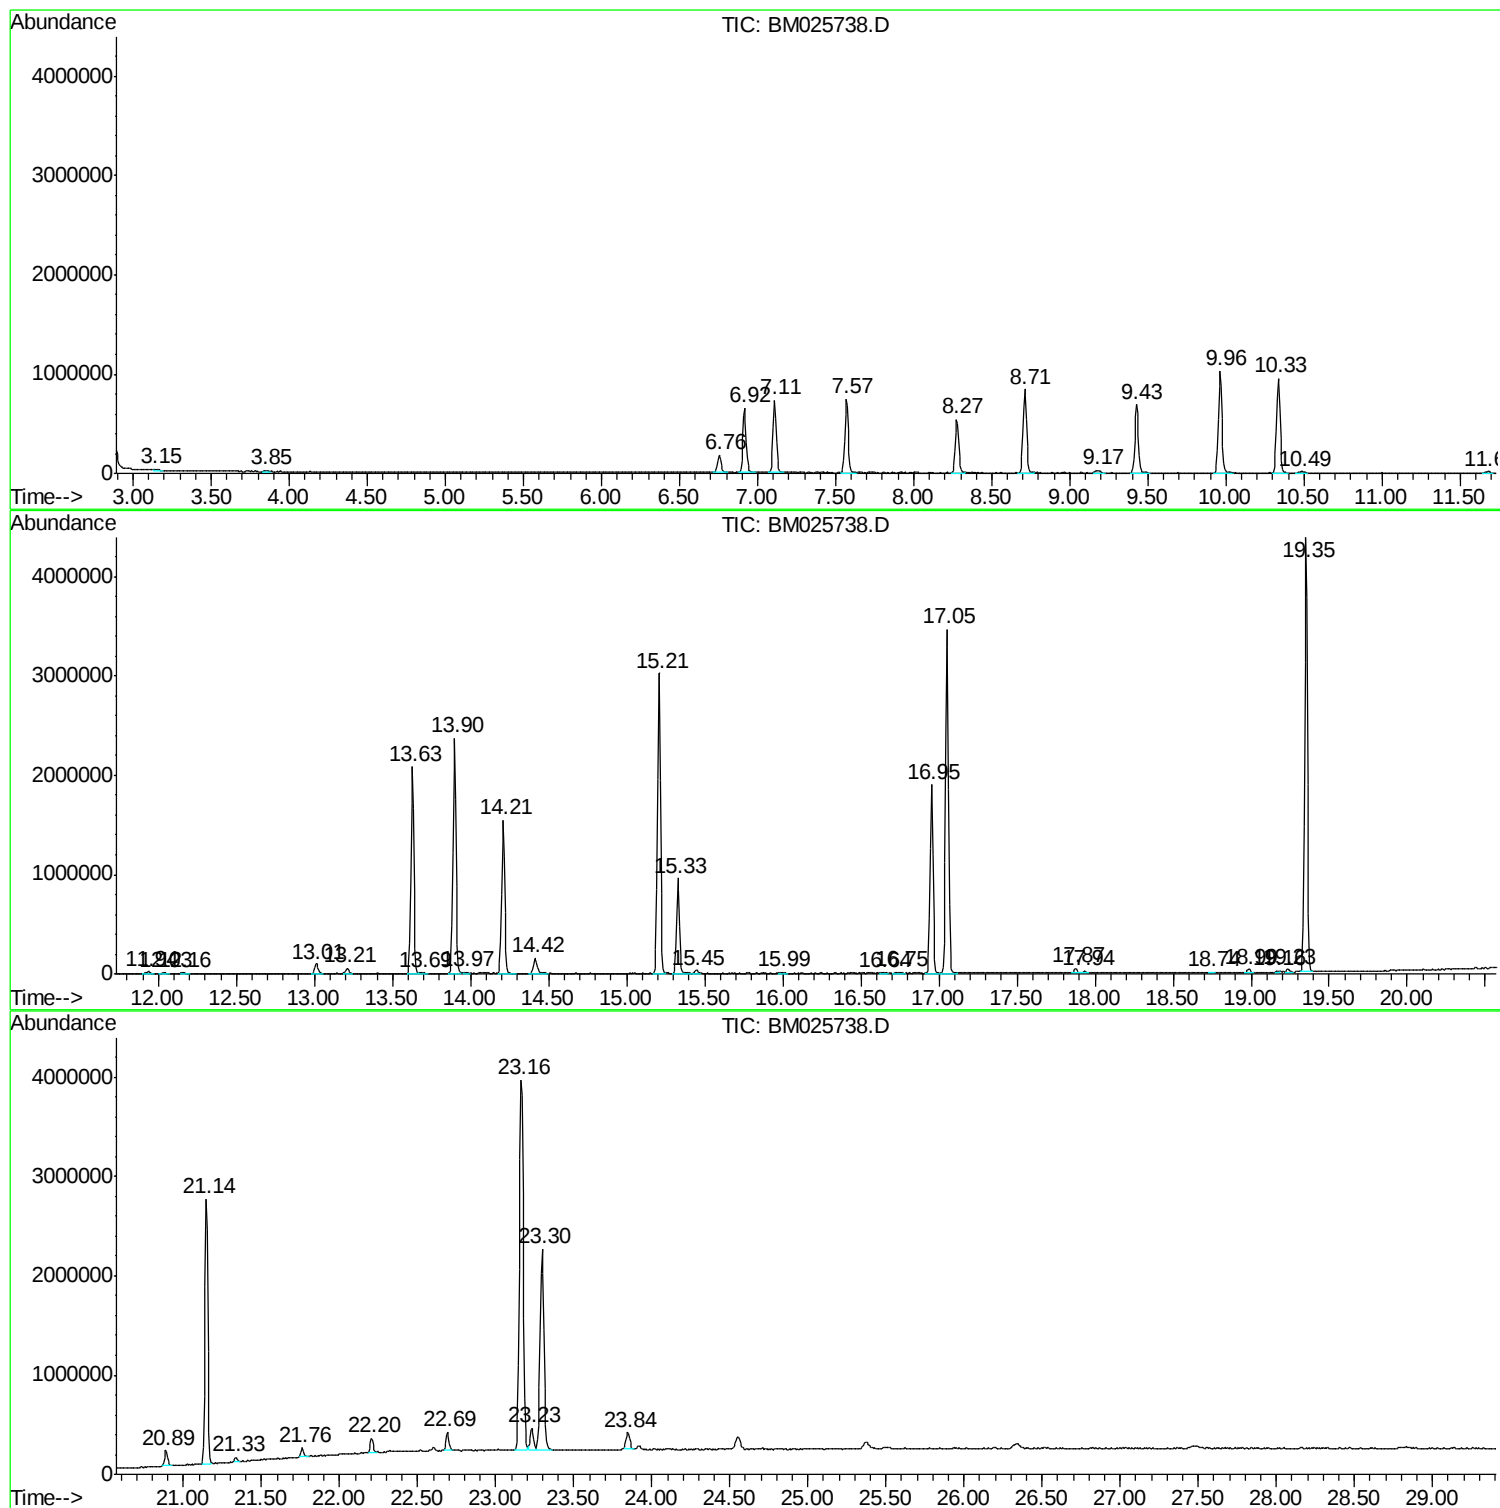

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025738.D
Acq On : 24 Mar 2020 20:44
Operator : CG/JU
Sample : L1940-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032320\
Data File : BM025738.D
Acq On : 24 Mar 2020 20:44
Operator : CG/JU
Sample : L1940-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0DA7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc